

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040730.D
 Acq On : 08 Jul 2023 08:30
 Operator : MA/JU
 Sample : PB153820BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK820

Quant Time: Jul 08 22:51:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	4526	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	16801	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.536	164	8235	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.286	188	15862	0.400	ng/ul	-0.01
17) Chrysene-d12	21.486	240	8306	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.89
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	19381	2.726	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	7613	0.323	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	15314	0.575	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.687	202	3077	0.081	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040730.D
Acq On : 08 Jul 2023 08:30
Operator : MA/JU
Sample : PB153820BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK820


Quant Time: Jul 08 22:51:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

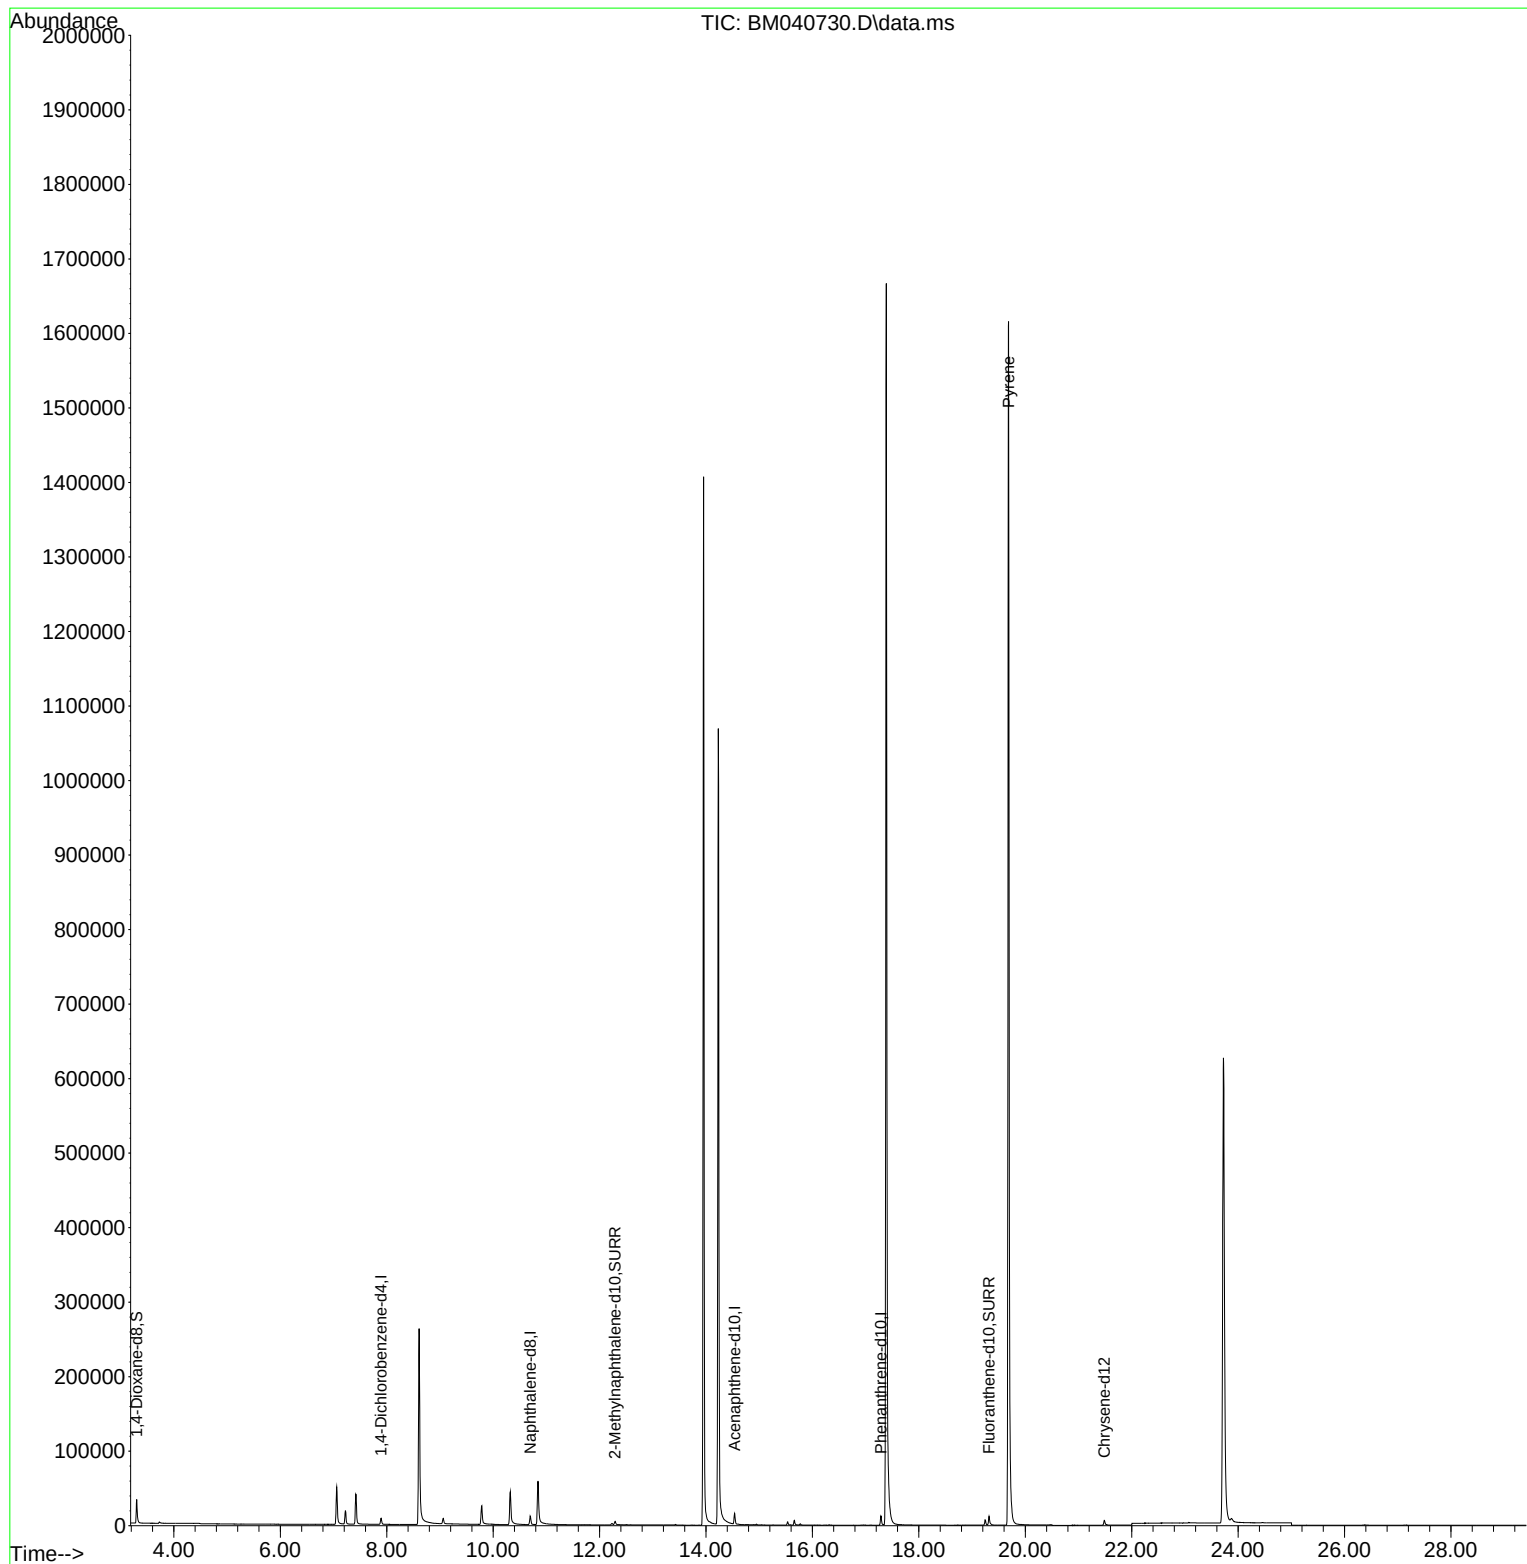

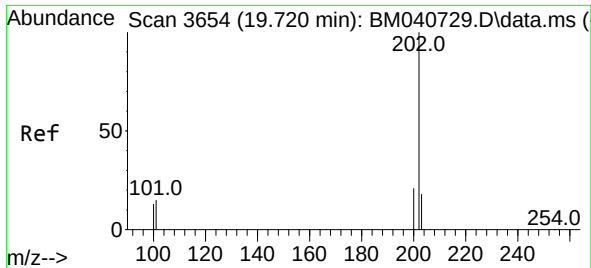

#20
 Pyrene
 Concen: 0.081 ng/ul
 RT: 19.687 min Scan# 30
 Delta R.T. -0.033 min
 Lab File: BM040730.D
 Acq: 08 Jul 2023 08:30

Instrument :
 BNA_M
 ClientSampleId :
 SBLK820

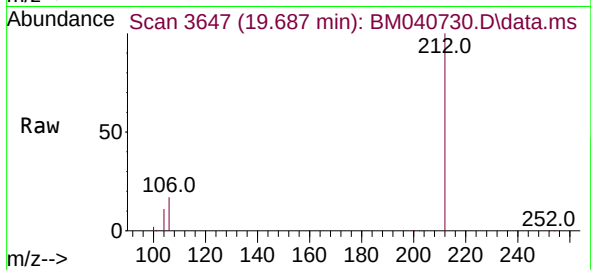

Tgt Ion:202 Resp: 3077
 Ion Ratio Lower Upper
 202 100
 101 177.5 12.6 18.8#
 100 1343.4 9.8 14.6#

