

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040731.D
 Acq On : 08 Jul 2023 09:07
 Operator : MA/JU
 Sample : 03332-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBTW9

Quant Time: Jul 08 22:56:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	4343	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	15973	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.537	164	7285	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.291	188	13564	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240	8116	0.400	ng/ul	0.00
23) Perylene-d12	23.877	264	7100	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	10602	1.554	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	2225	0.099	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	3072	0.118	ng/ul	0.00
Target Compounds						
					Qvalue	
24) Benzo(b)fluoranthene	23.152	252	711	0.026	ng/ul#	1
26) Benzo(a)pyrene	23.719	252	1195	0.048	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040731.D
Acq On : 08 Jul 2023 09:07
Operator : MA/JU
Sample : 03332-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBTW9


Quant Time: Jul 08 22:56:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

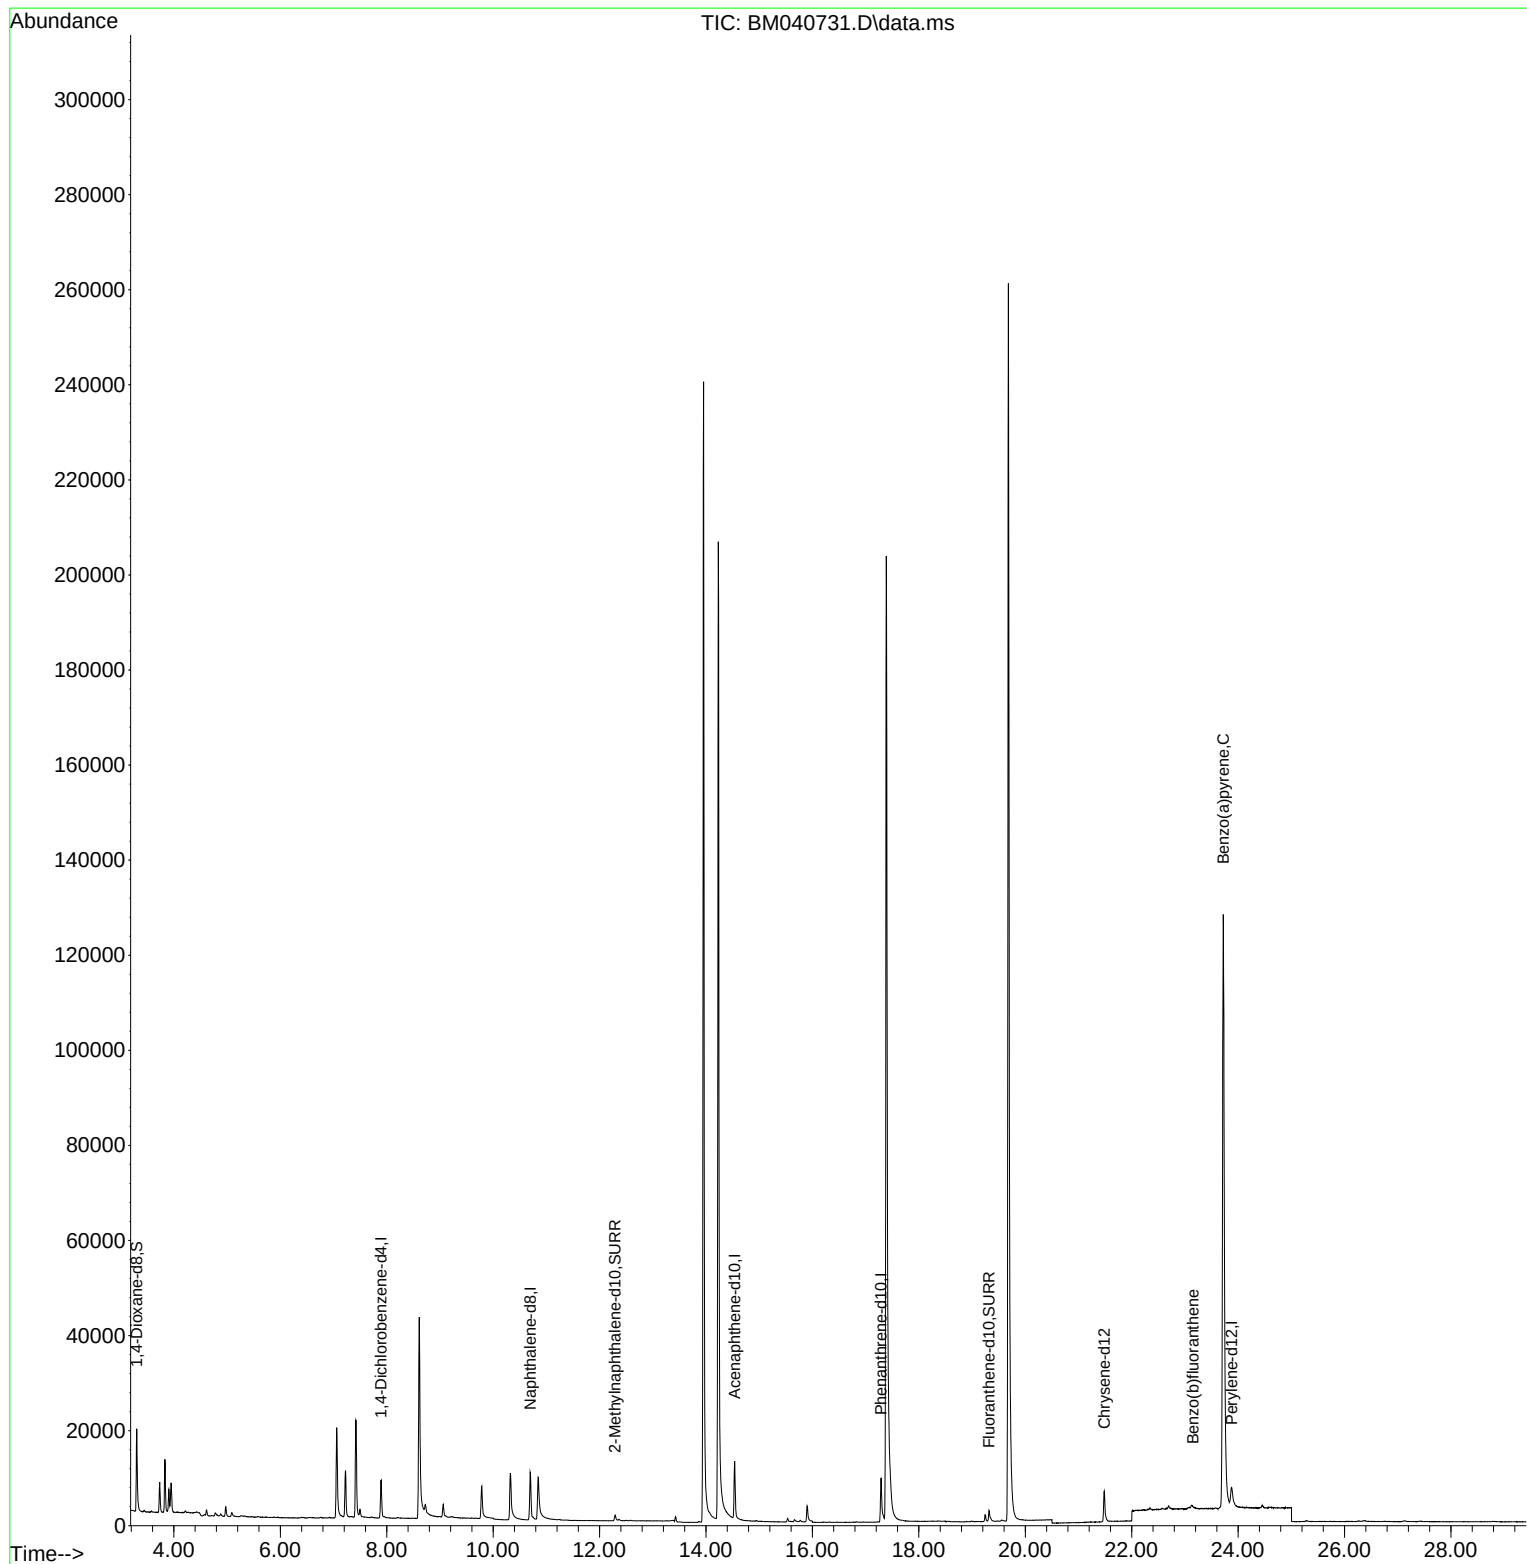



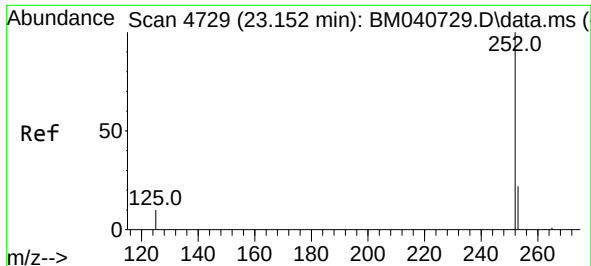


#24
Benzo(b)fluoranthene
Concen: 0.026 ng/ul
RT: 23.152 min Scan# 41
Delta R.T. -0.000 min
Lab File: BM040731.D
Acq: 08 Jul 2023 09:07

Instrument :
BNA_M
ClientSampleId :
YBTW9

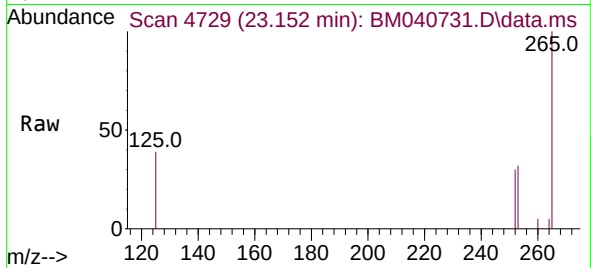

Tgt Ion:252 Resp: 711
Ion Ratio Lower Upper
252 100
253 107.3 0.0 52.8#
125 131.1 0.0 43.0#

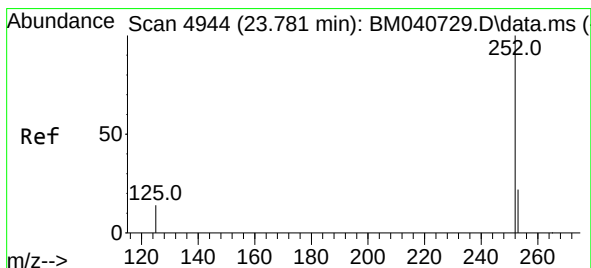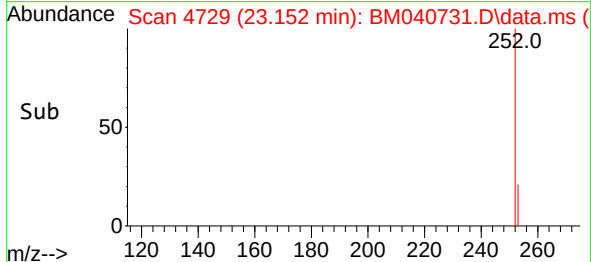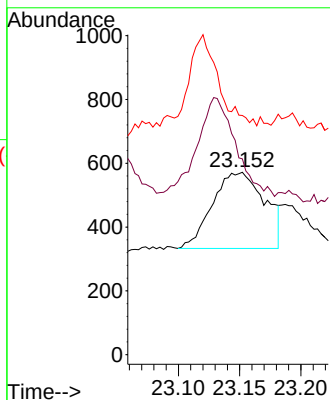

#26
Benzo(a)pyrene
Concen: 0.048 ng/ul
RT: 23.719 min Scan# 4923
Delta R.T. -0.061 min
Lab File: BM040731.D
Acq: 08 Jul 2023 09:07

Tgt Ion:252 Resp: 1195
Ion Ratio Lower Upper
252 100
253 86.4 22.9 34.3#
125 126.1 21.0 31.4#

