

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040733.D
 Acq On : 08 Jul 2023 10:22
 Operator : MA/JU
 Sample : 03332-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBTX2

Quant Time: Jul 08 22:57:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	3849	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	14157	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.537	164	7164	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.287	188	13916	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	9328	0.400	ng/ul	0.00
23) Perylene-d12	23.874	264	9381	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	30714	5.080	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	6353	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	9765	0.327	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.531	166	2546	0.088	ng/ul#	18
20) Pyrene	19.682	202	1825	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.719	252	2846	0.087	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040733.D
Acq On : 08 Jul 2023 10:22
Operator : MA/JU
Sample : 03332-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBTX2

Quant Time: Jul 08 22:57:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration




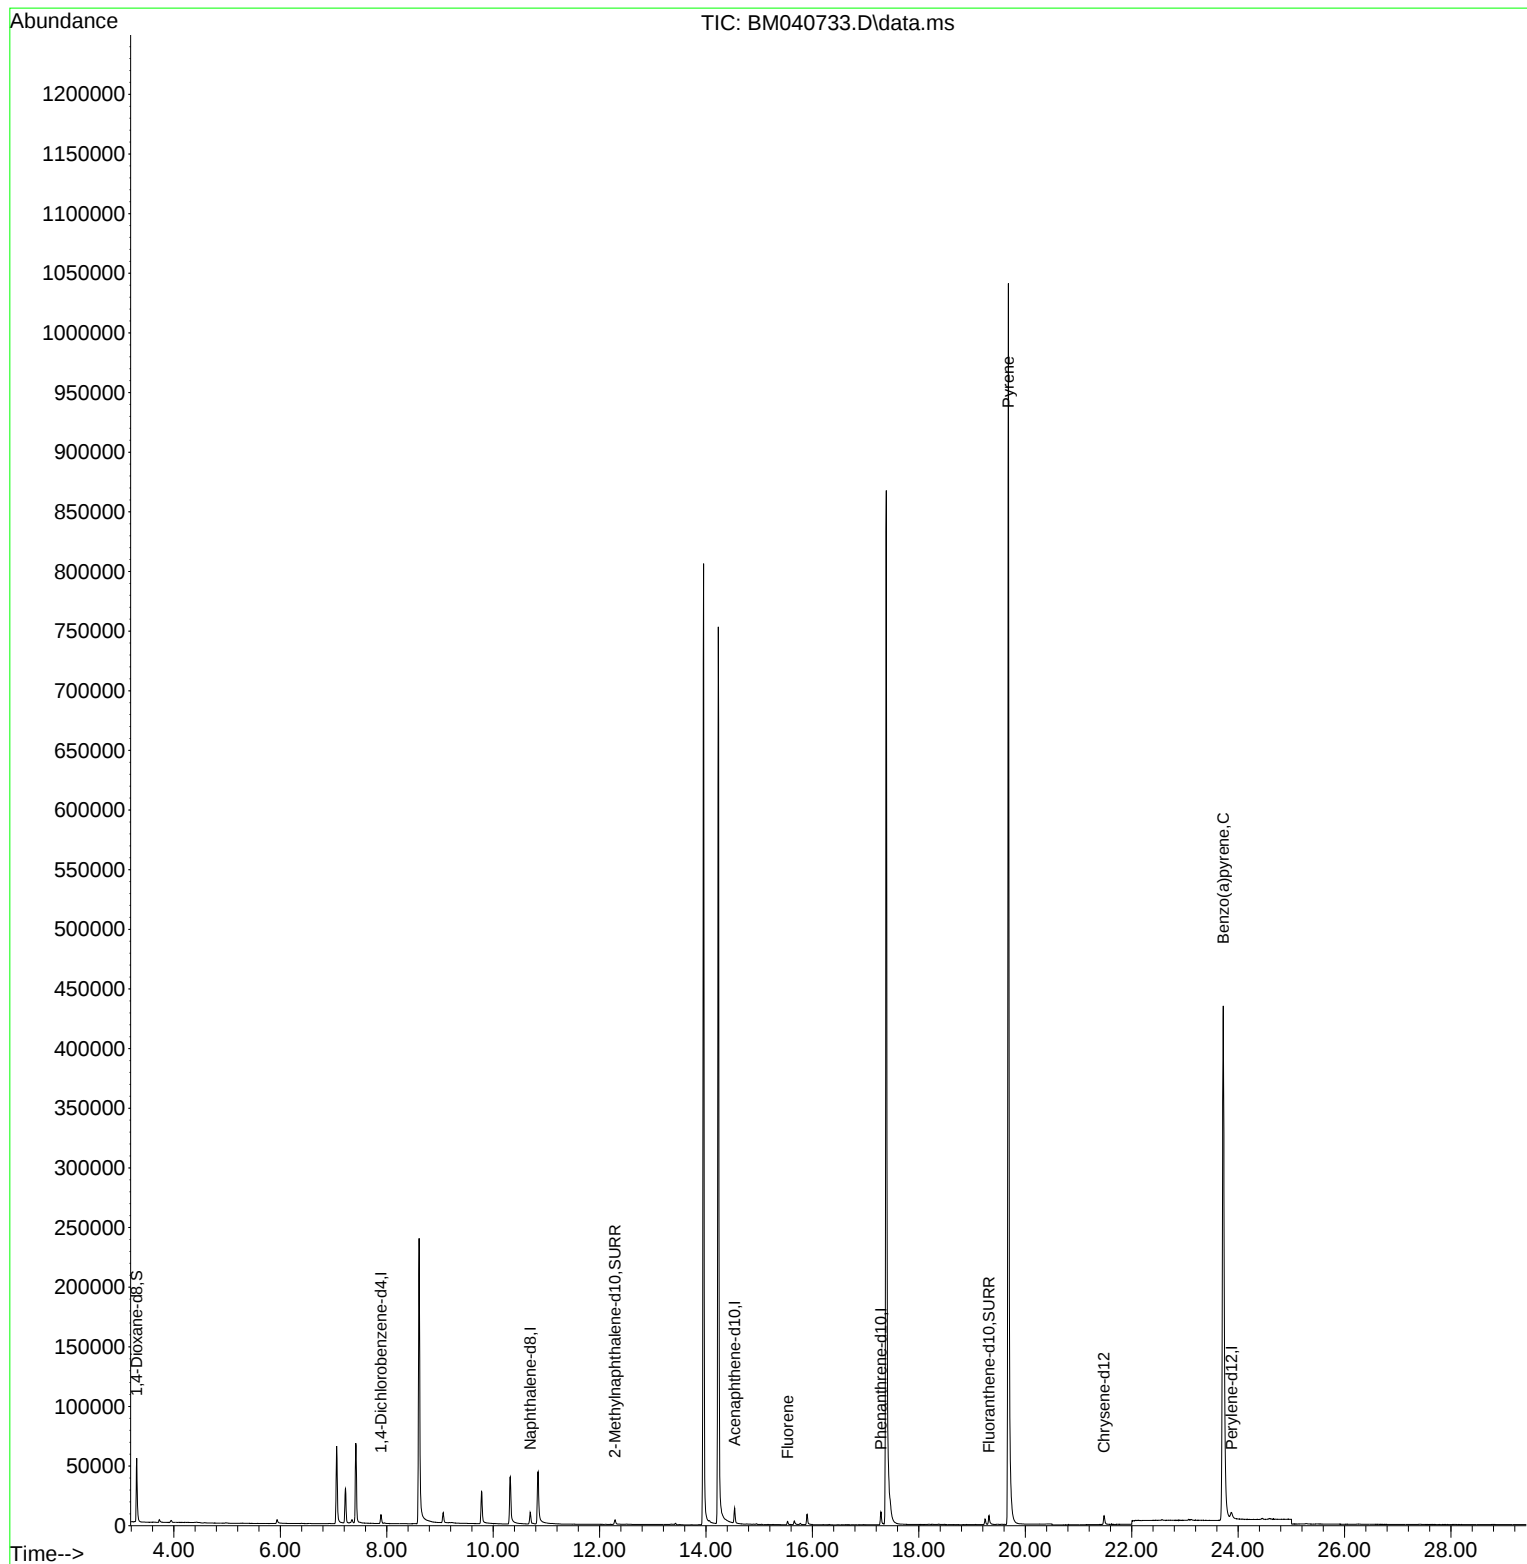


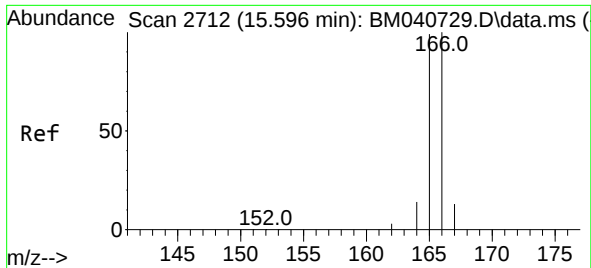

#12
Fluorene
Concen: 0.088 ng/ul
RT: 15.531 min Scan# 20
Delta R.T. -0.065 min
Lab File: BM040733.D
Acq: 08 Jul 2023 10:22




Instrument :
BNA_M
ClientSampleId :
YBTX2


Tgt Ion:166 Resp: 2546
Ion Ratio Lower Upper
166 100
165 12.4 79.6 119.4#
167 31.9 11.4 17.0#

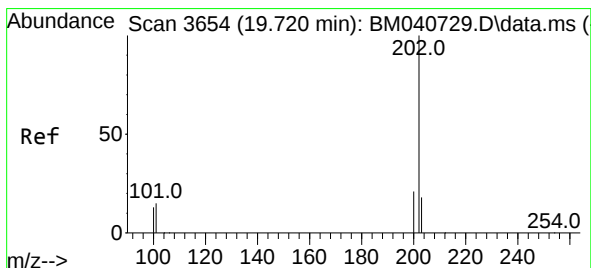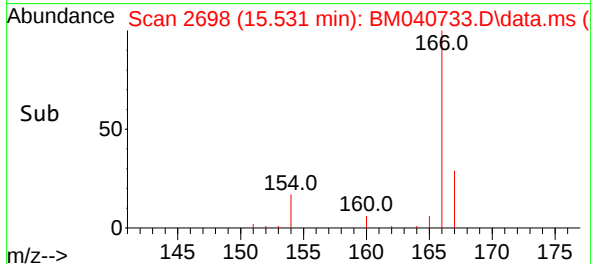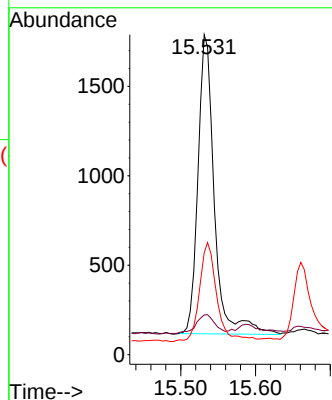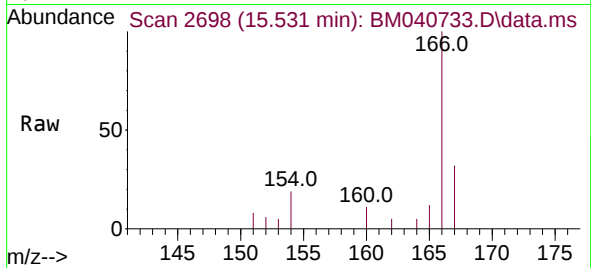

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.682 min Scan# 3646
Delta R.T. -0.037 min
Lab File: BM040733.D
Acq: 08 Jul 2023 10:22


Tgt Ion:202 Resp: 1825
Ion Ratio Lower Upper
202 100
101 188.7 12.6 18.8#
100 1387.3 9.8 14.6#

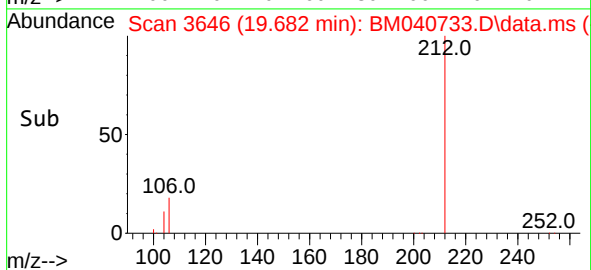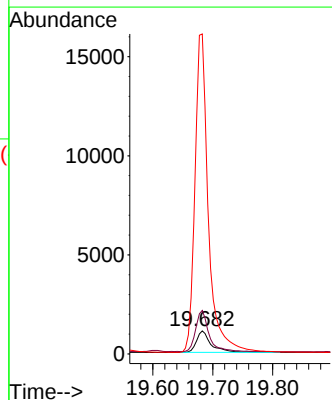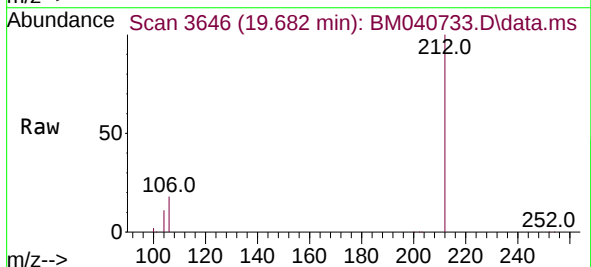

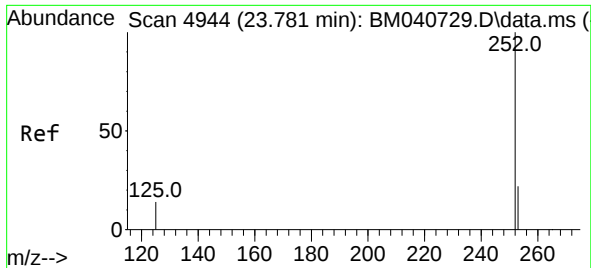

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.719 min Scan# 4923
Delta R.T. -0.061 min
Lab File: BM040733.D
Acq: 08 Jul 2023 10:22

Instrument :
BNA_M
ClientSampleId :
YBTX2

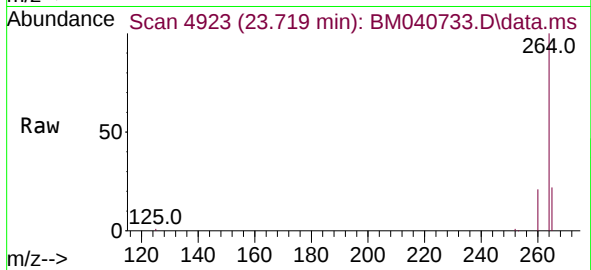

Tgt Ion:252 Resp: 2846
Ion Ratio Lower Upper
252 100
253 63.0 22.9 34.3#
125 118.4 21.0 31.4#

