

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040740.D
 Acq On : 08 Jul 2023 14:45
 Operator : MA/JU
 Sample : 03332-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBTX1

Quant Time: Jul 08 22:58:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	3750	0.400	ng/ul	0.00
4) Naphthalene-d8	10.696	136	14285	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.536	164	7176	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.286	188	13900	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	8805	0.400	ng/ul	0.00
23) Perylene-d12	23.874	264	7897	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	20953	3.557	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	4604	0.230	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	6846	0.243	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.531	166	1615	0.056	ng/ul#	21
20) Pyrene	19.682	202	1260	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.722	252	2036	0.074	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040740.D
Acq On : 08 Jul 2023 14:45
Operator : MA/JU
Sample : 03332-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBTX1

Quant Time: Jul 08 22:58:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration




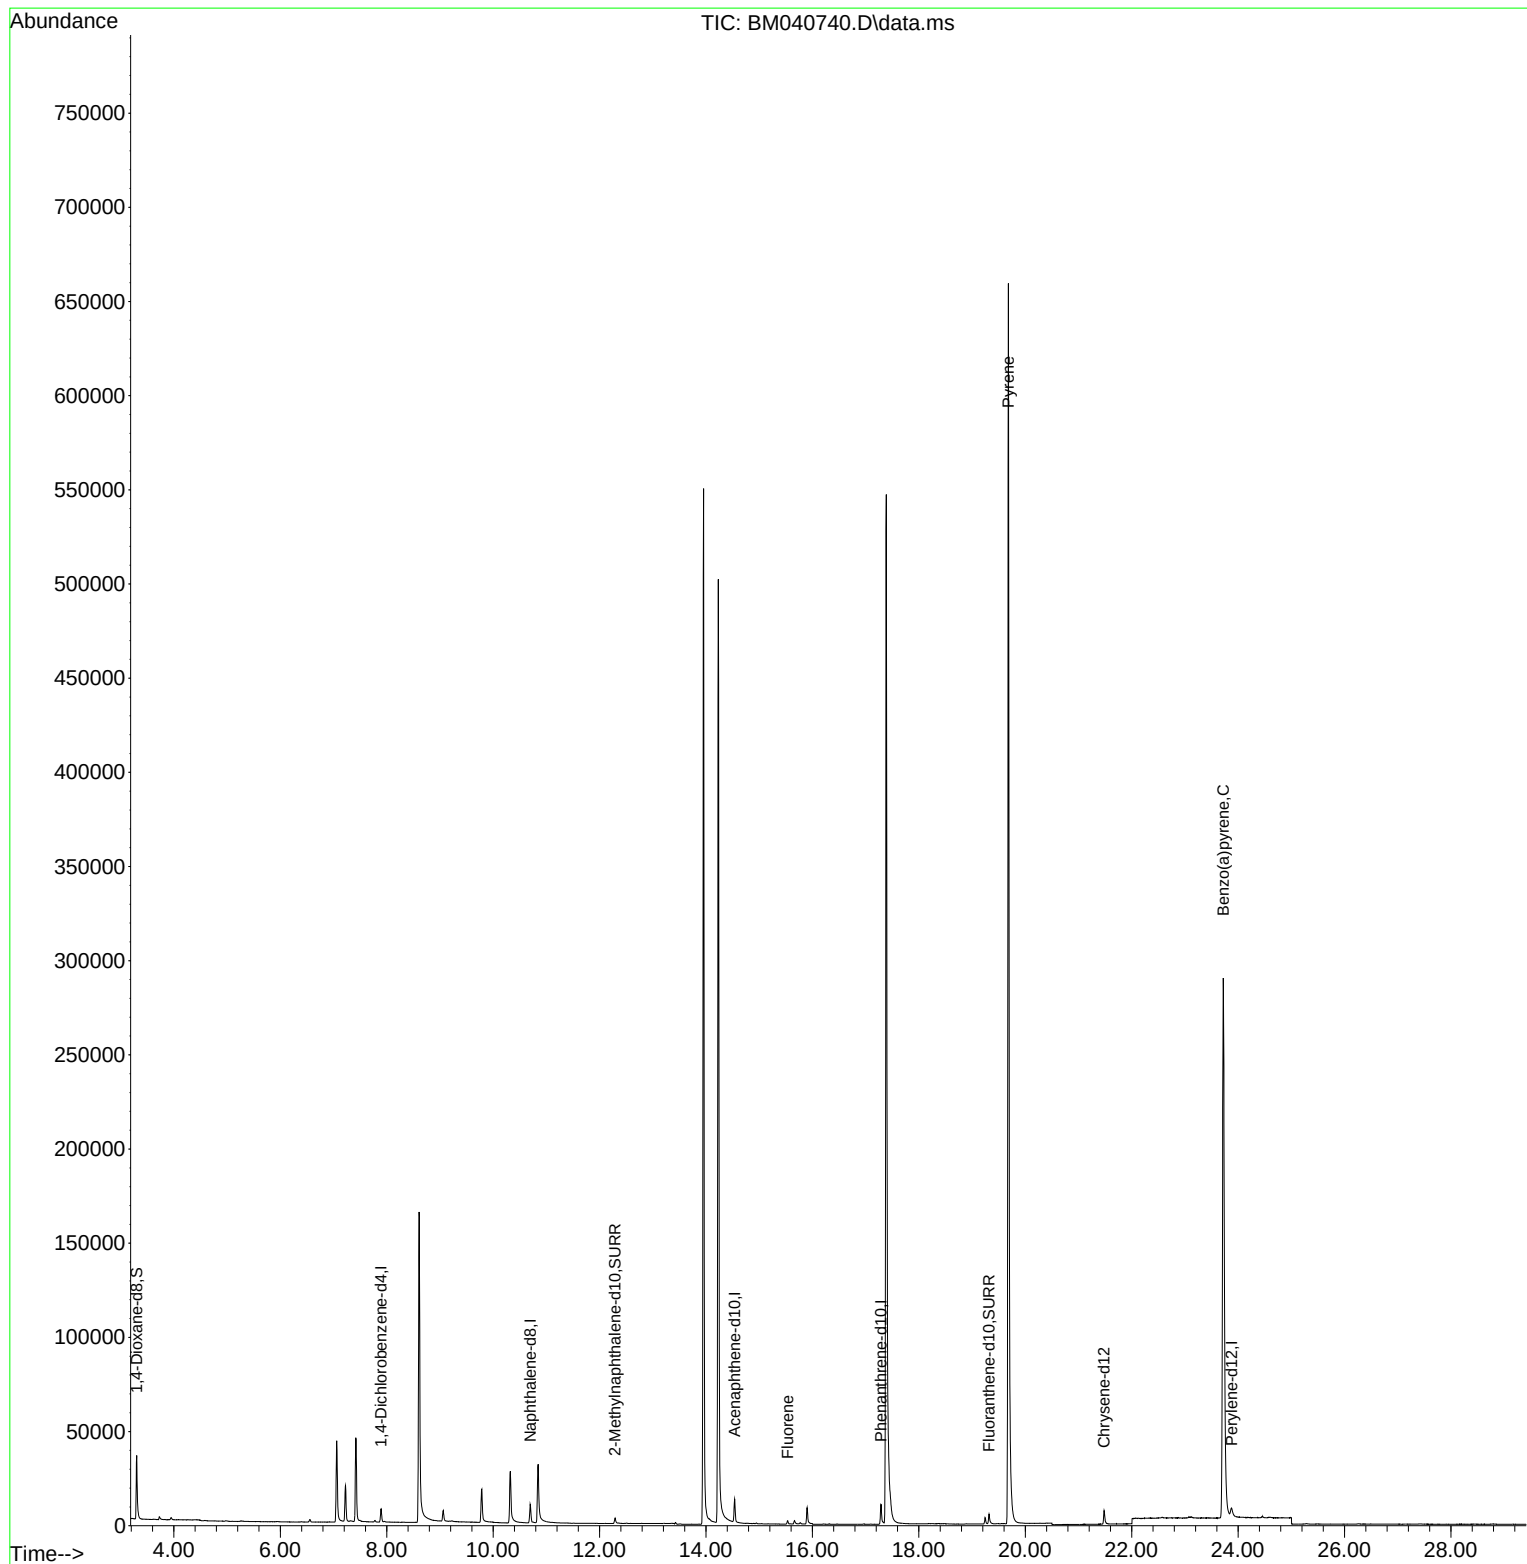


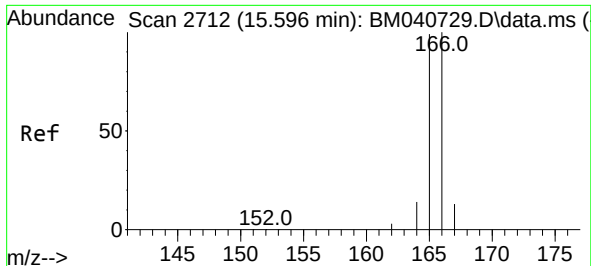

#12
 Fluorene
 Concen: 0.056 ng/ul
 RT: 15.531 min Scan# 2698
 Delta R.T. -0.065 min
 Lab File: BM040740.D
 Acq: 08 Jul 2023 14:45




Instrument :
 BNA_M
 ClientSampleId :
 YBTX1


Tgt Ion:166 Resp: 1615
 Ion Ratio Lower Upper
 166 100
 165 15.6 79.6 119.4#
 167 32.9 11.4 17.0#

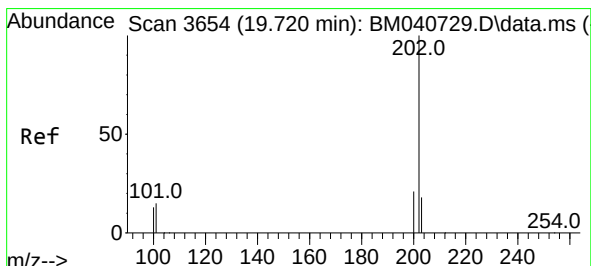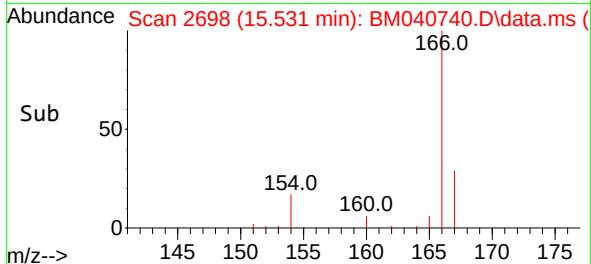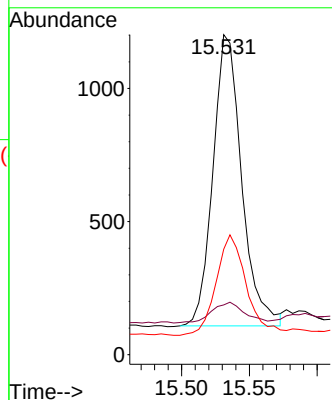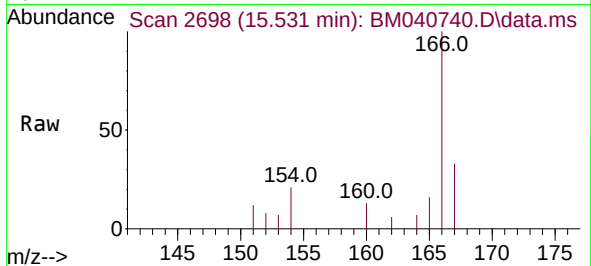

#20
 Pyrene
 Concen: 0.031 ng/ul
 RT: 19.682 min Scan# 3646
 Delta R.T. -0.037 min
 Lab File: BM040740.D
 Acq: 08 Jul 2023 14:45


Tgt Ion:202 Resp: 1260
 Ion Ratio Lower Upper
 202 100
 101 185.5 12.6 18.8#
 100 1368.5 9.8 14.6#

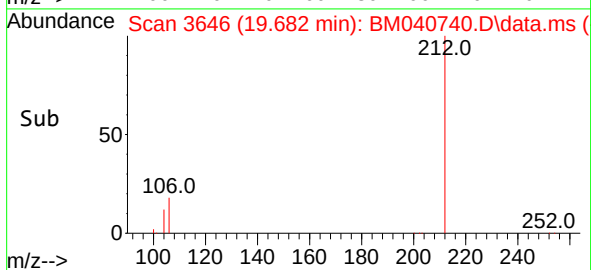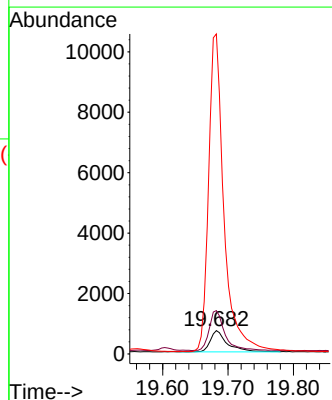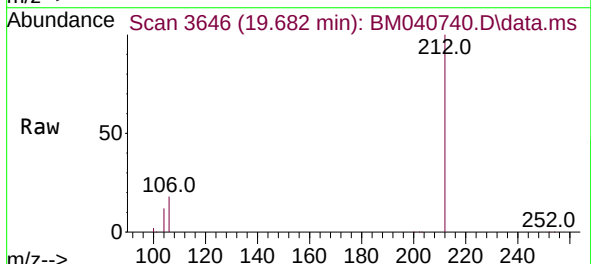

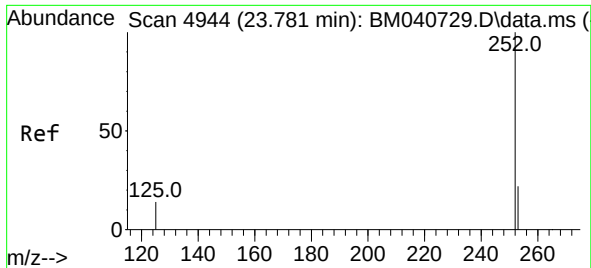

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.722 min Scan# 4944
Delta R.T. -0.059 min
Lab File: BM040740.D
Acq: 08 Jul 2023 14:45

Instrument :
BNA_M
ClientSampleId :
YBTX1

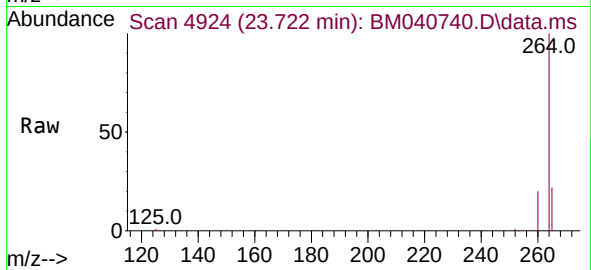

Tgt Ion:252 Resp: 2036
Ion Ratio Lower Upper
252 100
253 71.9 22.9 34.3#
125 119.4 21.0 31.4#

