

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040742.D
 Acq On : 08 Jul 2023 16:00
 Operator : MA/JU
 Sample : 03348-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBTY4

Quant Time: Jul 08 22:58:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.891	152	4192	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	15235	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.537	164	7487	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.287	188	14446	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	8877	0.400	ng/ul	0.00
23) Perylene-d12	23.871	264	8310	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	22703	3.448	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	5384	0.252	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	8330	0.293	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.682	202	1706	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.719	252	2423	0.084	ng/ul#	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040742.D
Acq On : 08 Jul 2023 16:00
Operator : MA/JU
Sample : 03348-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBTY4

Quant Time: Jul 08 22:58:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration




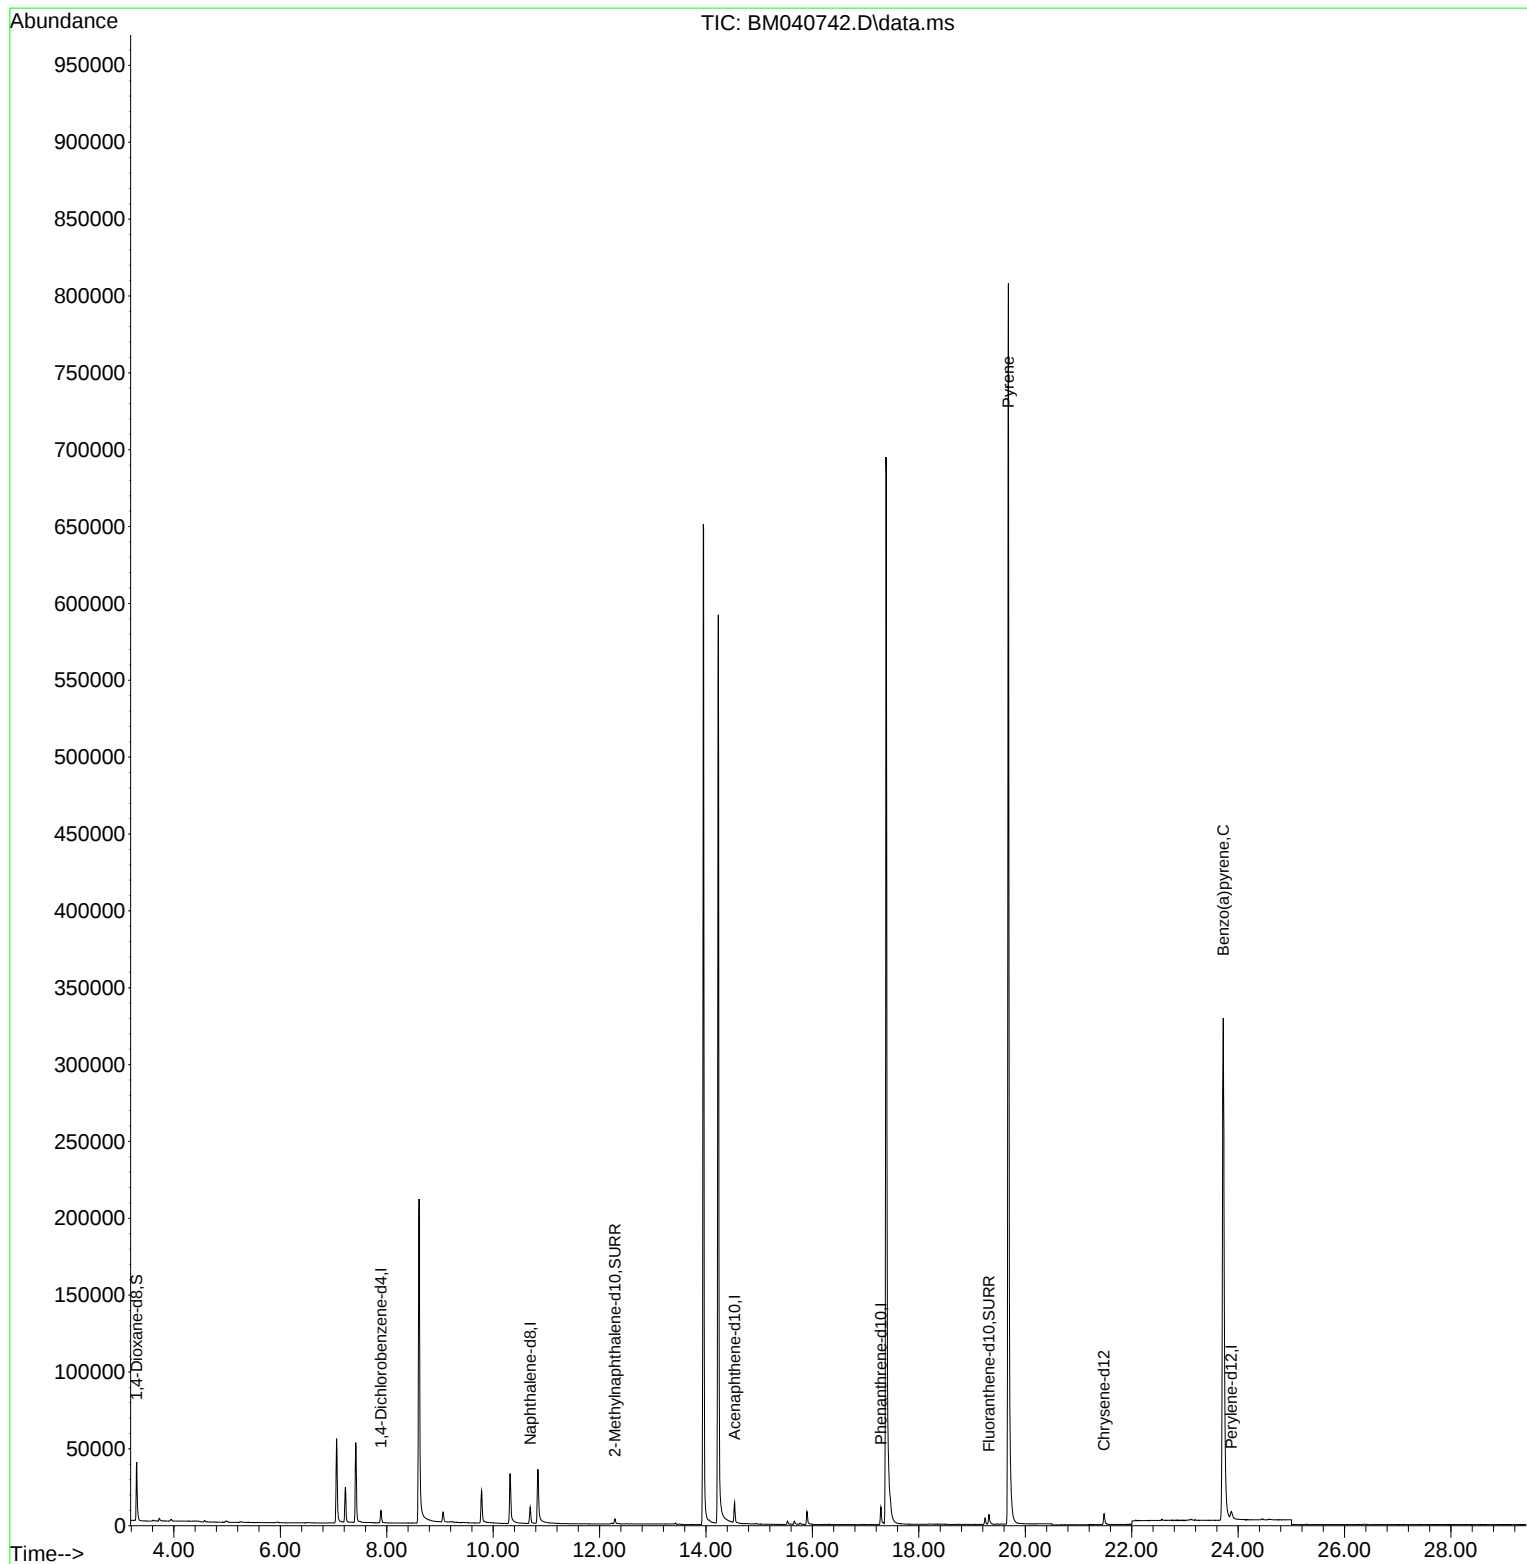


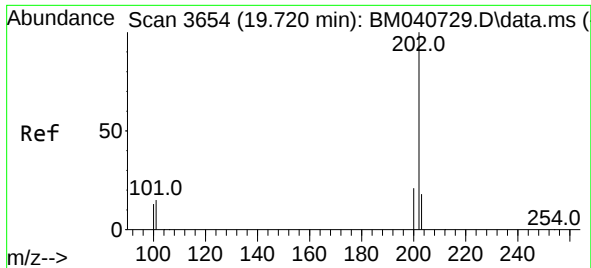

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.682 min Scan# 3646
Delta R.T. -0.037 min
Lab File: BM040742.D
Acq: 08 Jul 2023 16:00

Instrument :
BNA_M
ClientSampleId :
YBTY4

Tgt Ion:202 Resp: 1706
Ion Ratio Lower Upper
202 100
101 191.4 12.6 18.8#
100 1398.9 9.8 14.6#

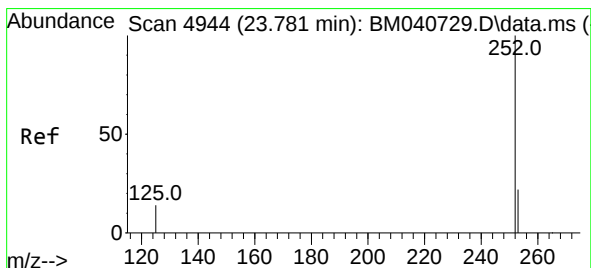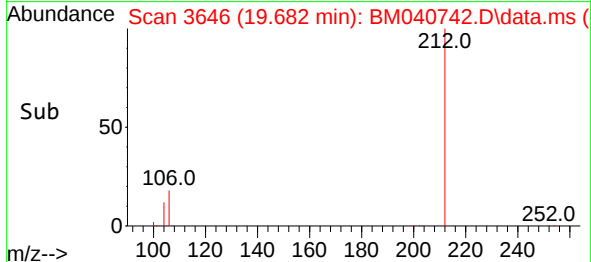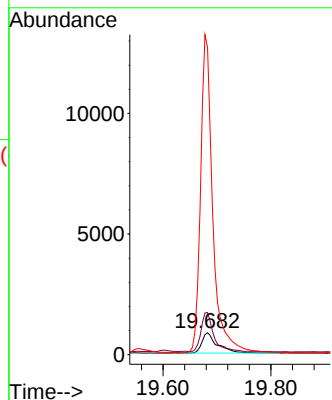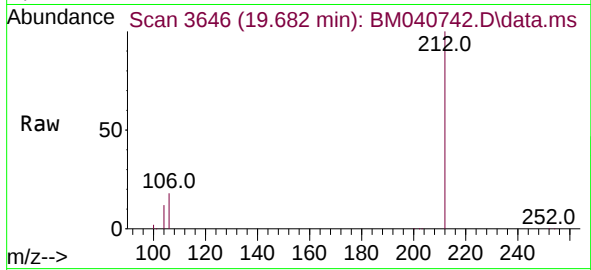

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.719 min Scan# 4923
Delta R.T. -0.061 min
Lab File: BM040742.D
Acq: 08 Jul 2023 16:00

Tgt Ion:252 Resp: 2423
Ion Ratio Lower Upper
252 100
253 63.0 22.9 34.3#
125 83.8 21.0 31.4#

