

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040743.D
 Acq On : 08 Jul 2023 16:38
 Operator : MA/JU
 Sample : 03348-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBW20

Quant Time: Jul 08 22:59:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.891	152	3791	0.400	ng/ul	0.00
4) Naphthalene-d8	10.696	136	14074	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.536	164	7900	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.286	188	14935	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	9054	0.400	ng/ul	0.00
23) Perylene-d12	23.871	264	8786	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	22584	3.793	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	7784	0.395	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	15613	0.538	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.682	202	3089	0.075	ng/ul#	1
26) Benzo(a)pyrene	23.719	252	4489	0.147	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040743.D
Acq On : 08 Jul 2023 16:38
Operator : MA/JU
Sample : 03348-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBW20

Quant Time: Jul 08 22:59:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration




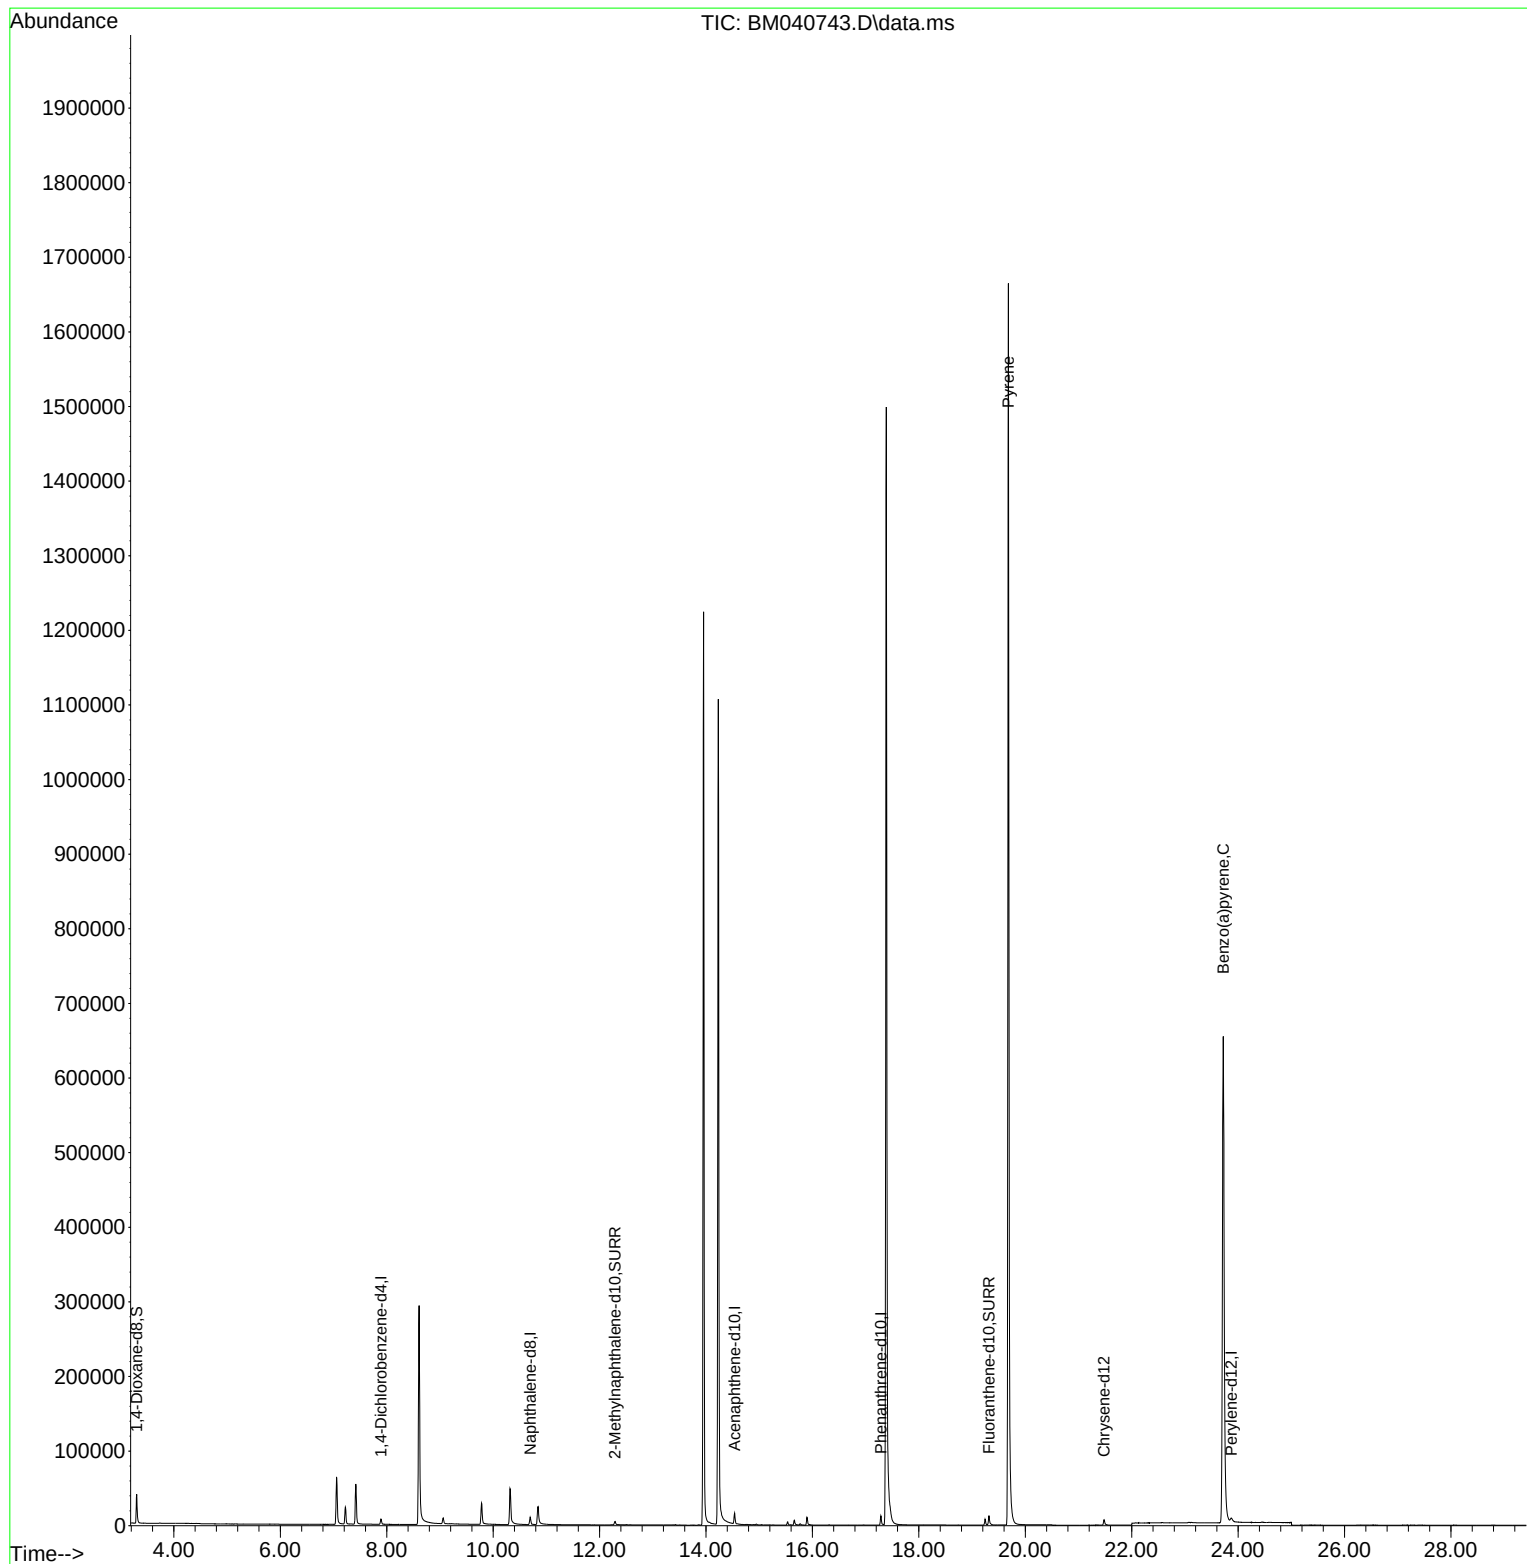


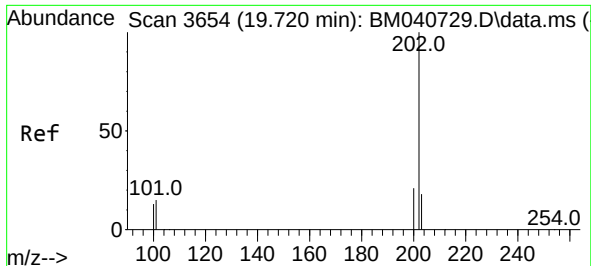

#20
Pyrene
Concen: 0.075 ng/ul
RT: 19.682 min Scan# 3089
Delta R.T. -0.037 min
Lab File: BM040743.D
Acq: 08 Jul 2023 16:38

Instrument :
BNA_M
ClientSampleId :
YBW20

Tgt Ion:202 Resp: 3089
Ion Ratio Lower Upper
202 100
101 182.2 12.6 18.8#
100 1380.9 9.8 14.6#

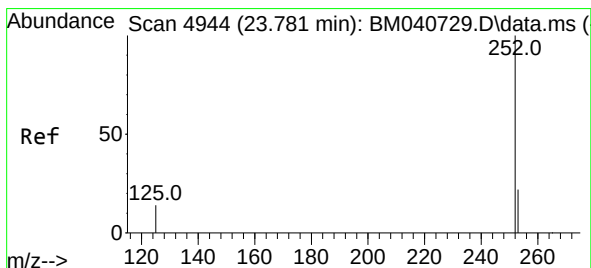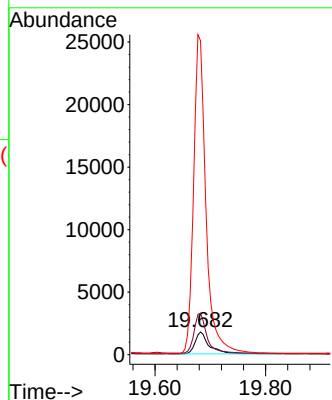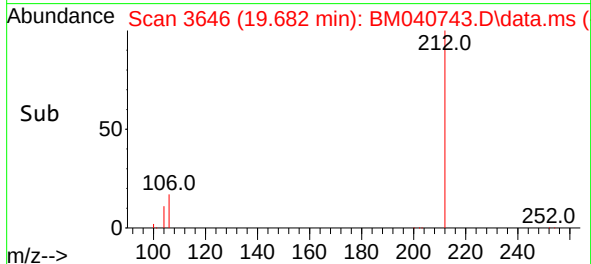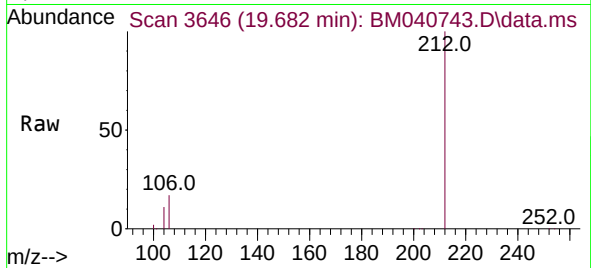

#26
Benzo(a)pyrene
Concen: 0.147 ng/ul
RT: 23.719 min Scan# 4923
Delta R.T. -0.062 min
Lab File: BM040743.D
Acq: 08 Jul 2023 16:38

Tgt Ion:252 Resp: 4489
Ion Ratio Lower Upper
252 100
253 53.0 22.9 34.3#
125 61.6 21.0 31.4#

