

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040746.D
 Acq On : 08 Jul 2023 19:08
 Operator : MA/JU
 Sample : PB153845BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK845

Quant Time: Jul 08 23:31:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.891	152	4468	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	16521	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.537	164	9019	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.287	188	17499	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	10398	0.400	ng/ul	0.00
23) Perylene-d12	23.871	264	10170	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	16430	2.341	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	6345	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	15164	0.455	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.682	202	3195	0.067	ng/ul#	1
26) Benzo(a)pyrene	23.716	252	4729	0.133	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040746.D
Acq On : 08 Jul 2023 19:08
Operator : MA/JU
Sample : PB153845BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK845

Quant Time: Jul 08 23:31:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

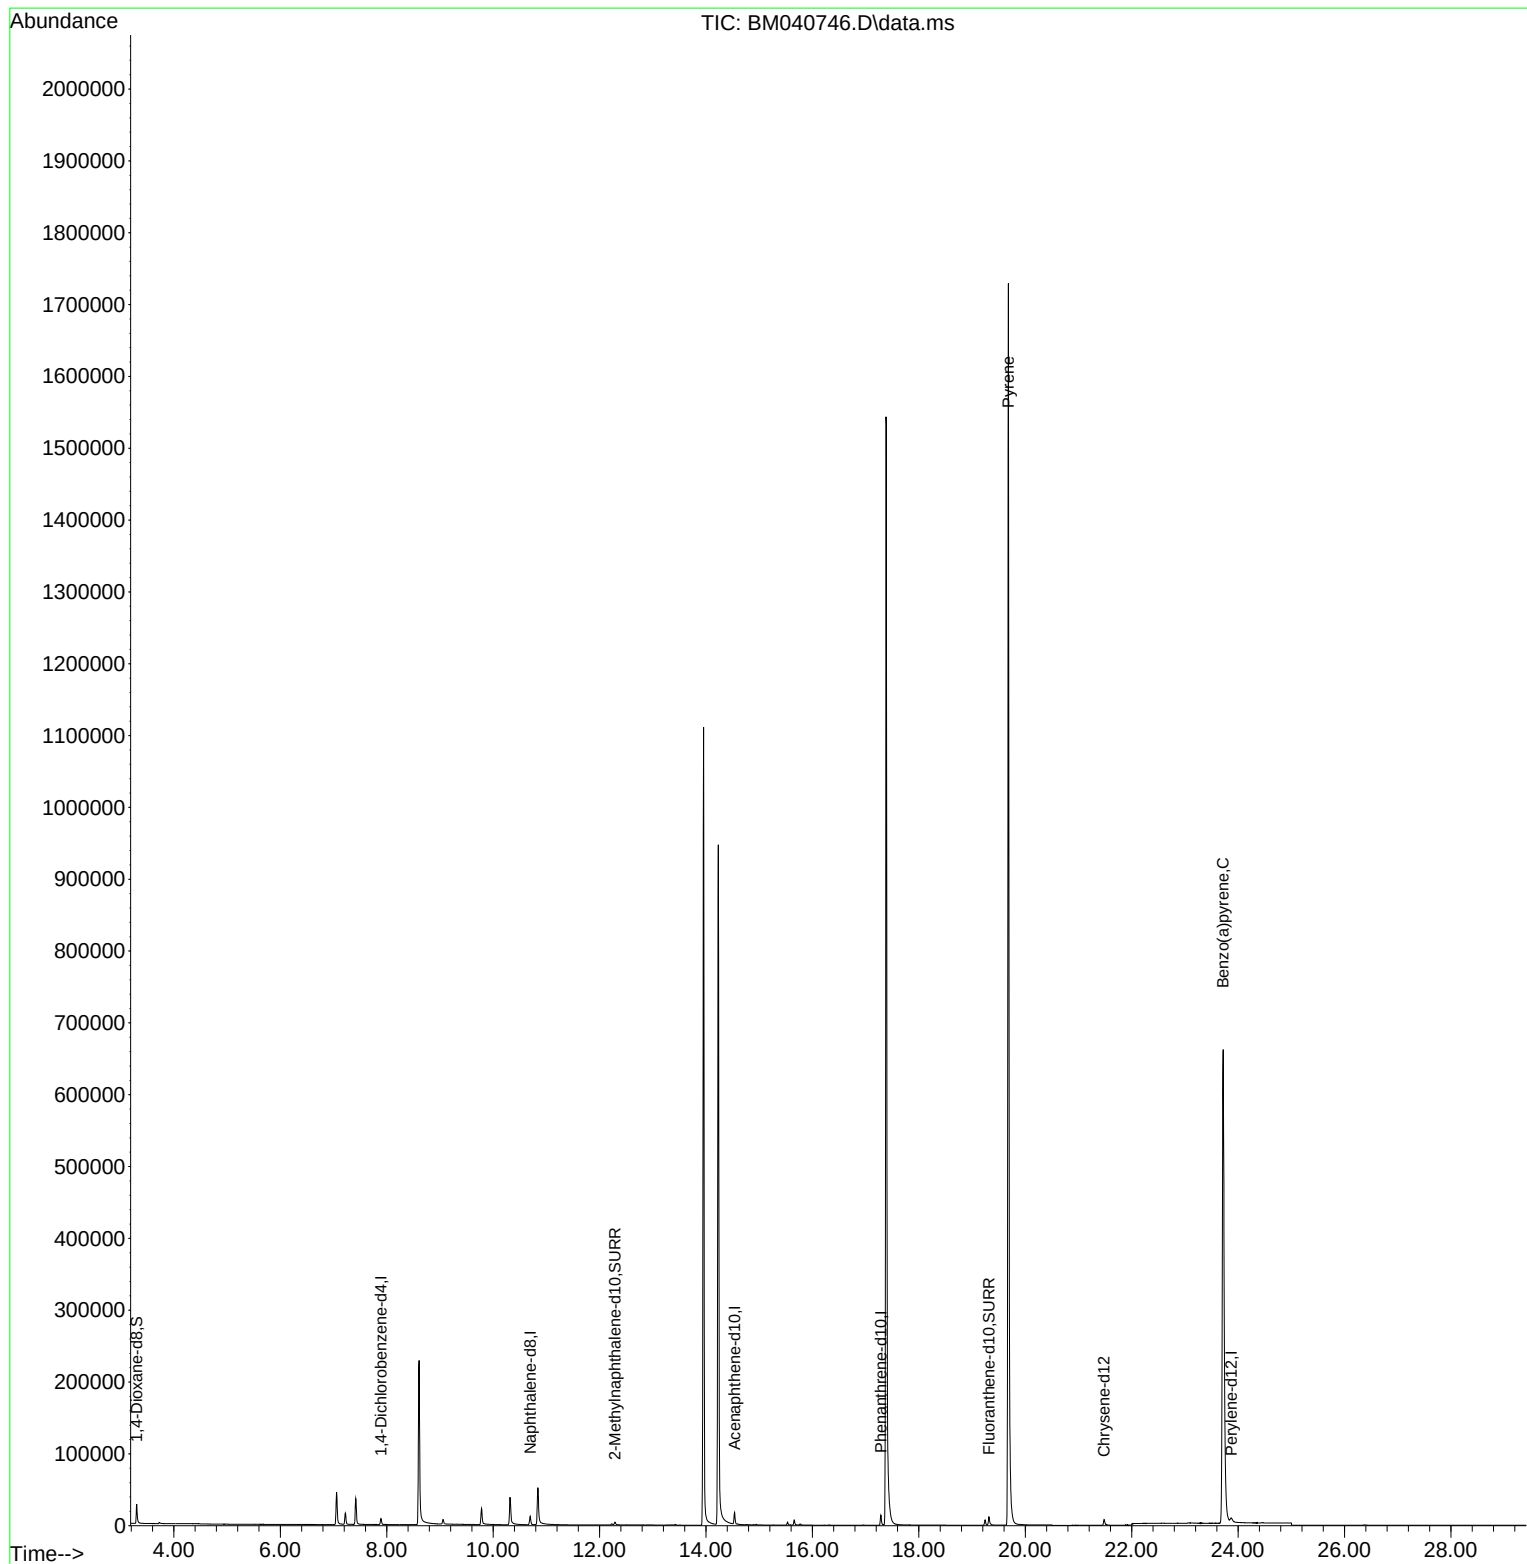

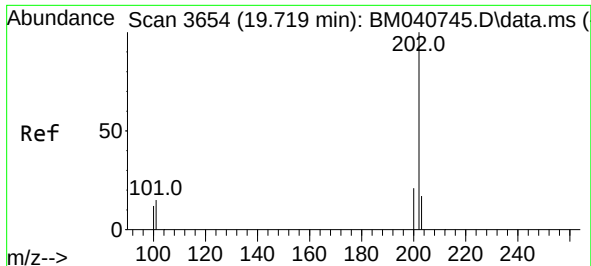

#20

Pyrene

Concen: 0.067 ng/ul

RT: 19.682 min Scan# 3

Delta R.T. -0.037 min

Lab File: BM040746.D

Acq: 08 Jul 2023 19:08

Instrument :





BNA_M

ClientSampleId :

SBLK845

Tgt Ion:202 Resp: 3195

Ion	Ratio	Lower	Upper
202	100		
101	187.1	12.6	18.8#
100	1423.1	9.8	14.6#

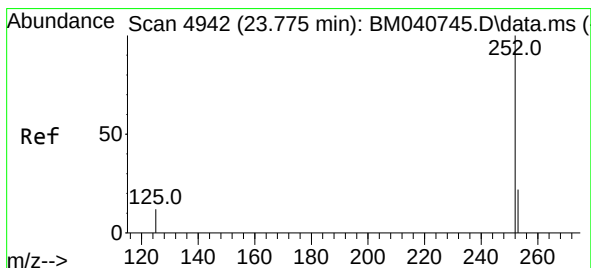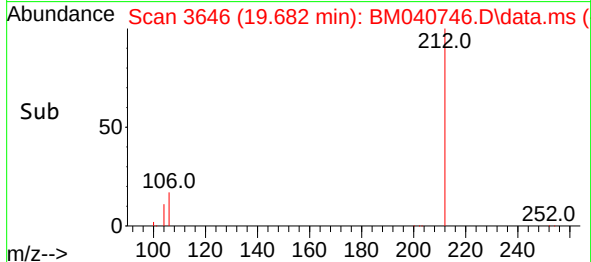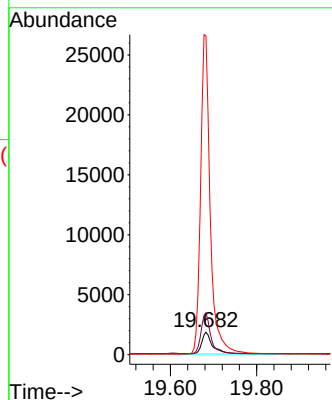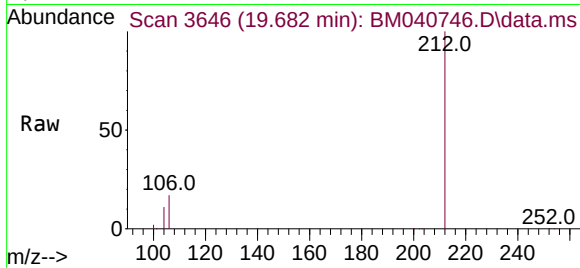

#26

Benzo(a)pyrene

Concen: 0.133 ng/ul

RT: 23.716 min Scan# 4922

Delta R.T. -0.064 min

Lab File: BM040746.D

Acq: 08 Jul 2023 19:08

Tgt Ion:252 Resp: 4729

Ion	Ratio	Lower	Upper
252	100		
253	50.6	22.9	34.3#
125	56.0	21.0	31.4#

