

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040752.D
 Acq On : 08 Jul 2023 22:54
 Operator : MA/JU
 Sample : 03348-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBTX8

Quant Time: Jul 08 23:33:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.891	152	4755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.696	136	17401	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.536	164	8758	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.286	188	16357	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	10415	0.400	ng/ul	-0.01
23) Perylene-d12	23.871	264	9737	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	26885	3.599	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	6622	0.271	ng/ul	0.00
18) Fluoranthene-d10	19.315	212	10173	0.305	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.531	166	2550	0.072	ng/ul#	17
20) Pyrene	19.682	202	1846	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.713	252	2641	0.078	ng/ul#	4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040752.D
Acq On : 08 Jul 2023 22:54
Operator : MA/JU
Sample : 03348-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBTX8

Quant Time: Jul 08 23:33:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

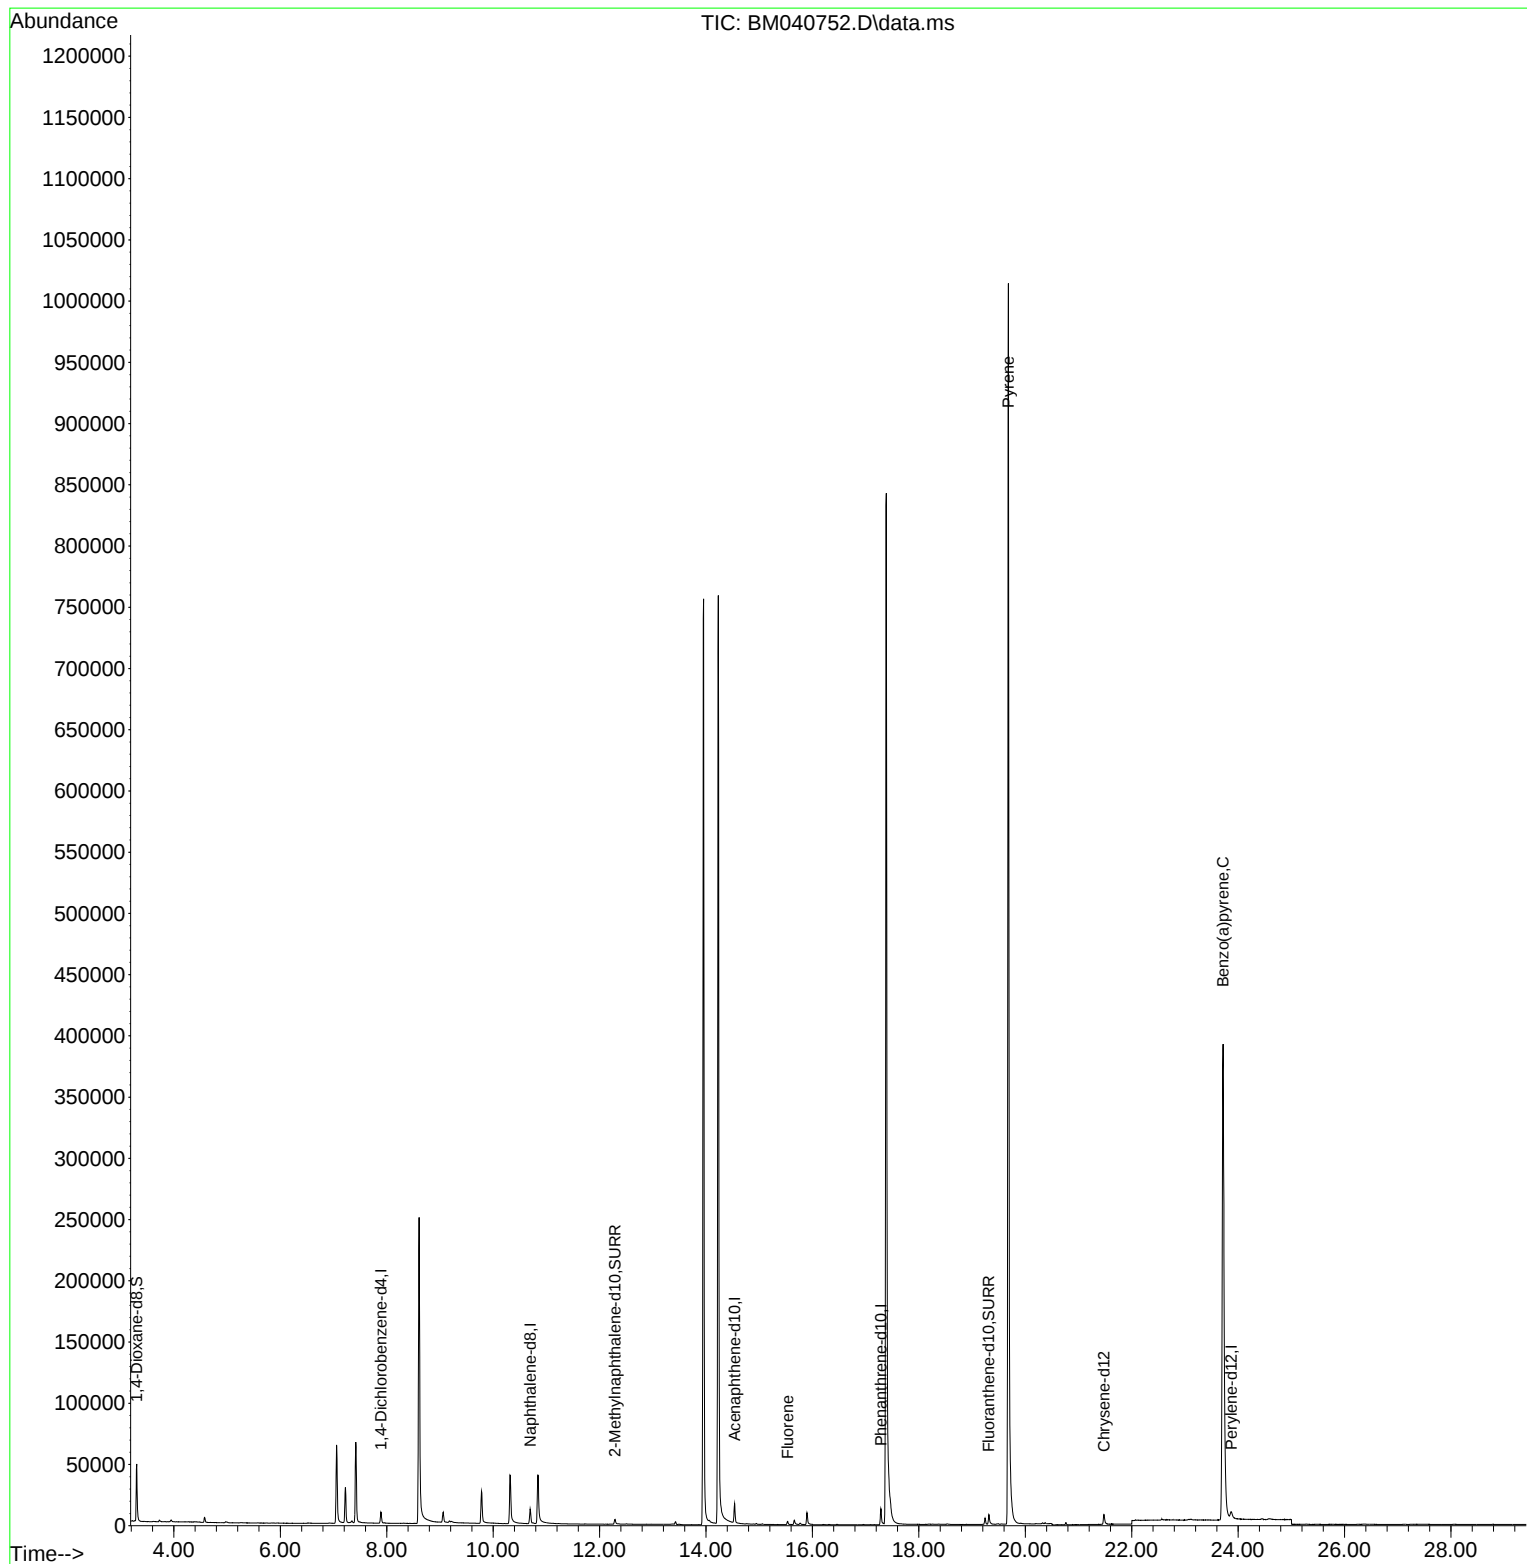

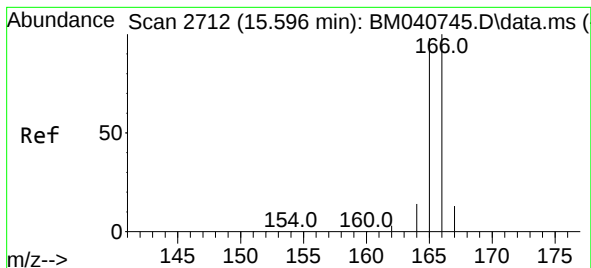

#12

Fluorene

Concen: 0.072 ng/ul

RT: 15.531 min Scan# 2

Delta R.T. -0.065 min

Lab File: BM040752.D

Acq: 08 Jul 2023 22:54

Instrument :

BNA_M

ClientSampleId :

YBTX8





Tgt Ion:166 Resp: 2550

Ion Ratio Lower Upper

166 100

165 12.3 79.6 119.4#

167 33.7 11.4 17.0#

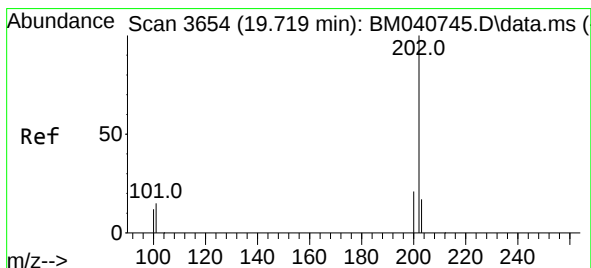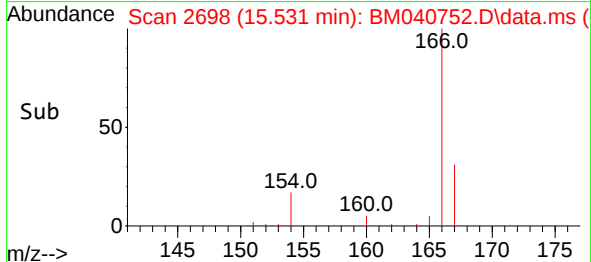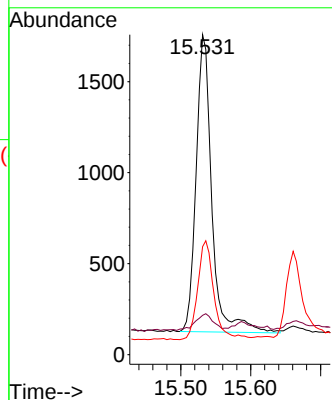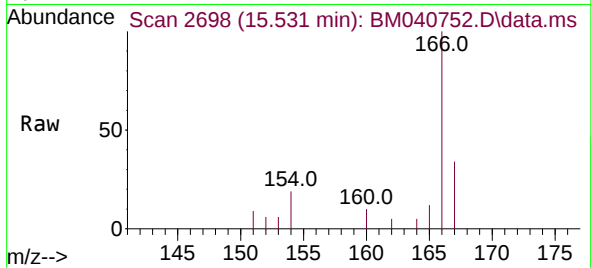

#20

Pyrene

Concen: 0.039 ng/ul

RT: 19.682 min Scan# 3646

Delta R.T. -0.037 min

Lab File: BM040752.D

Acq: 08 Jul 2023 22:54




Tgt Ion:202 Resp: 1846


Ion Ratio Lower Upper

202 100

101 174.7 12.6 18.8#


100 1277.4 9.8 14.6#

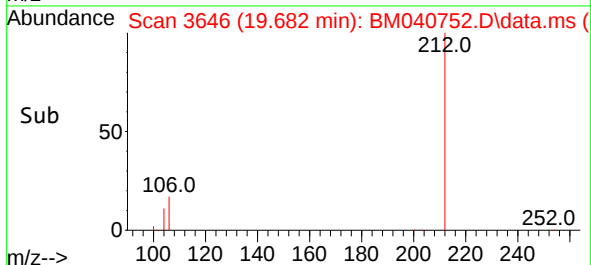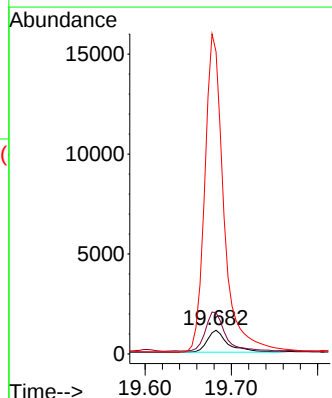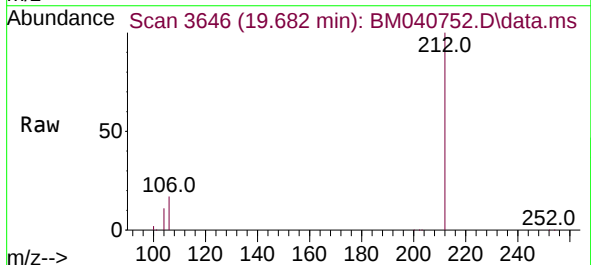

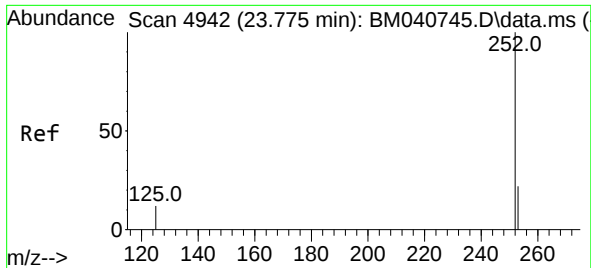

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.713 min Scan# 4942
Delta R.T. -0.067 min
Lab File: BM040752.D
Acq: 08 Jul 2023 22:54

Instrument :
BNA_M
ClientSampleId :
YBTX8

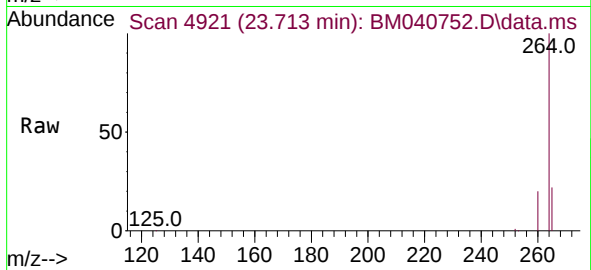

Tgt Ion:252 Resp: 2641
Ion Ratio Lower Upper
252 100
253 67.5 22.9 34.3#
125 88.5 21.0 31.4#

