




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040730.D
 Acq On : 08 Jul 2023 08:30
 Operator : MA/JU
 Sample : PB153820BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK820

Manual IntegrationsAPPROVED

Quant Time: Jul 08 22:51:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

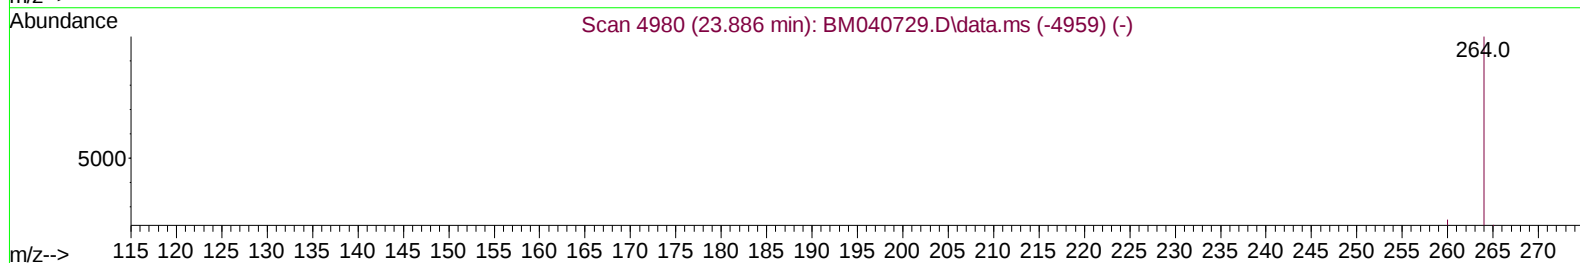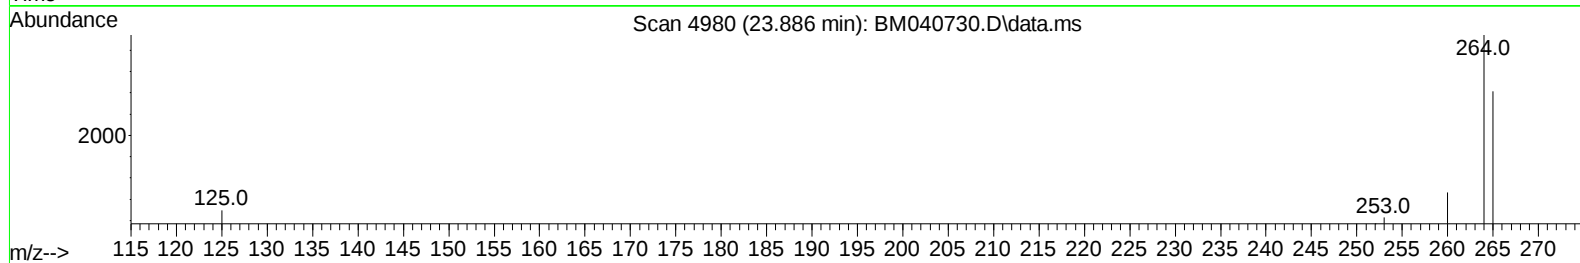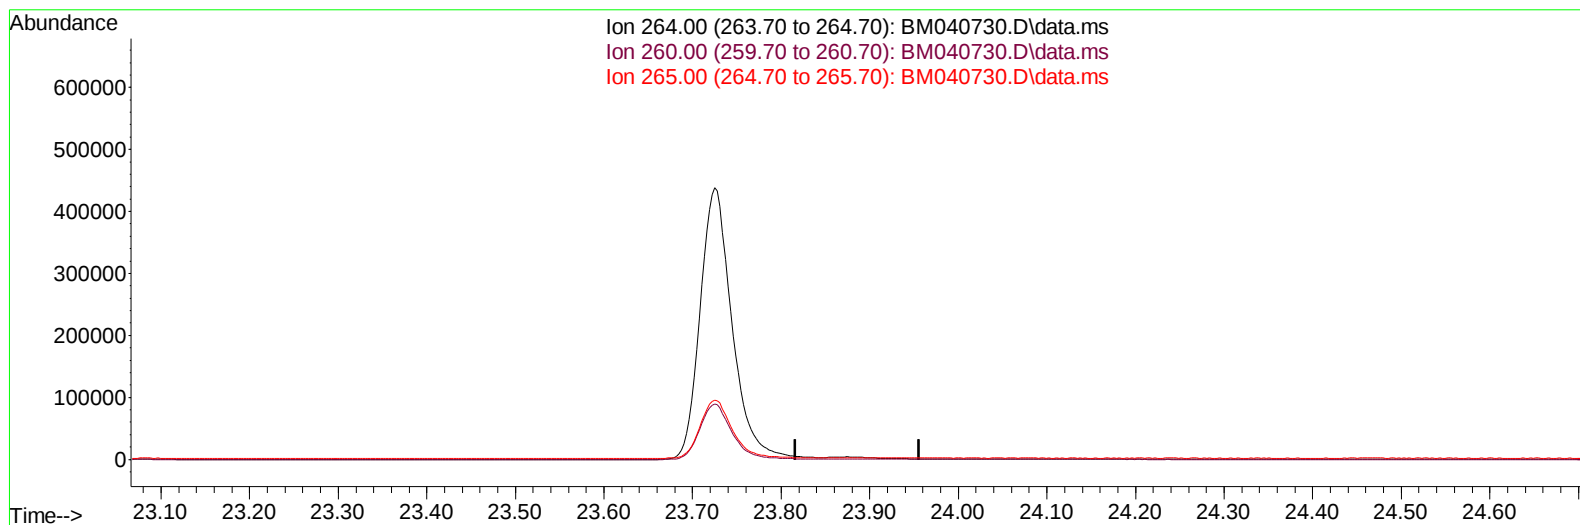

TIC: BM040730.D\data.ms

(23) Perylene-d12 (I)

23.886min (-23.886) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040730.D
Acq On : 08 Jul 2023 08:30
Operator : MA/JU
Sample : PB153820BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK820

Manual IntegrationsAPPROVED

Quant Time: Jul 08 22:51:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

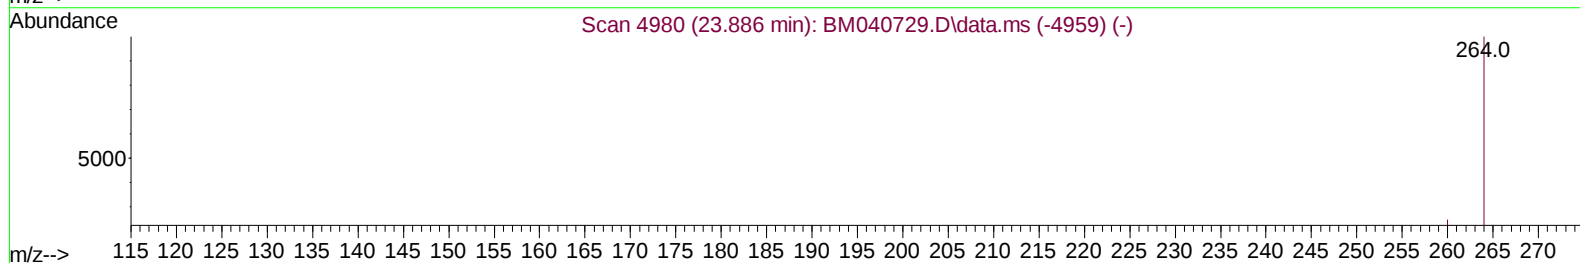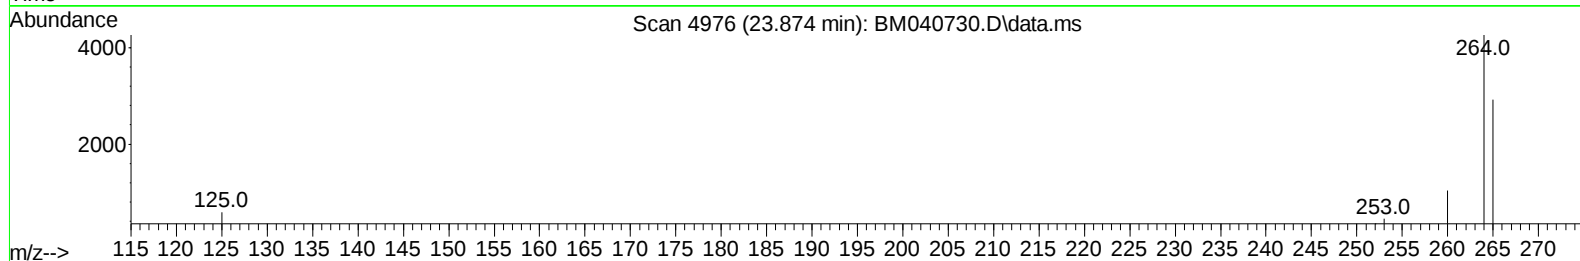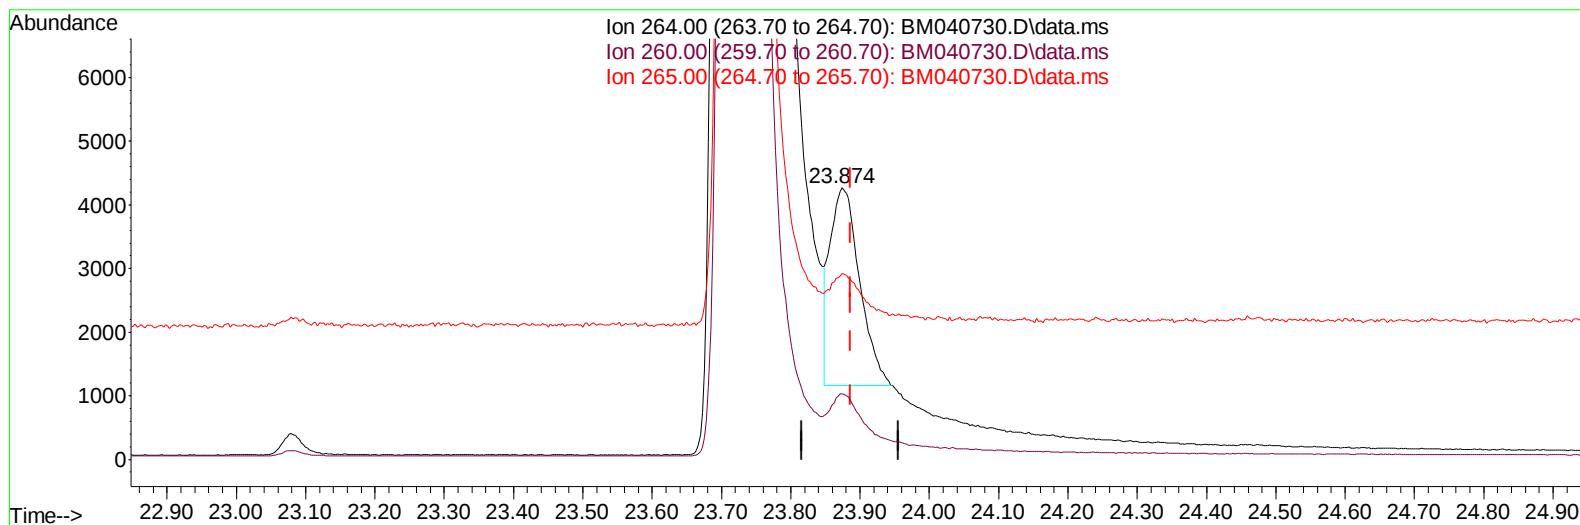

TIC: BM040730.D\data.ms

(23) Perylene-d12 (I)

23.874min (-0.012) 0.40 ng/ul m

response 9264

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	24.16
265.00	79.20	68.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040730.D
 Acq On : 08 Jul 2023 08:30
 Operator : MA/JU
 Sample : PB153820BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK820

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

Quant Time: Jul 08 22:51:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	4526	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	16801	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.536	164	8235	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.286	188	15862	0.400	ng/ul	-0.01
17) Chrysene-d12	21.486	240	8306	0.400	ng/ul	0.00
23) Perylene-d12	23.874	264	9264m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	19381	2.726	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	7613	0.323	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	15314	0.575	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040730.D
Acq On : 08 Jul 2023 08:30
Operator : MA/JU
Sample : PB153820BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK820

Manual IntegrationsAPPROVED

Quant Time: Jul 08 22:51:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

