




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040763.D
 Acq On : 09 Jul 2023 06:25
 Operator : MA/JU
 Sample : PB153845BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK845

Manual IntegrationsAPPROVED

Quant Time: Jul 09 14:08:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

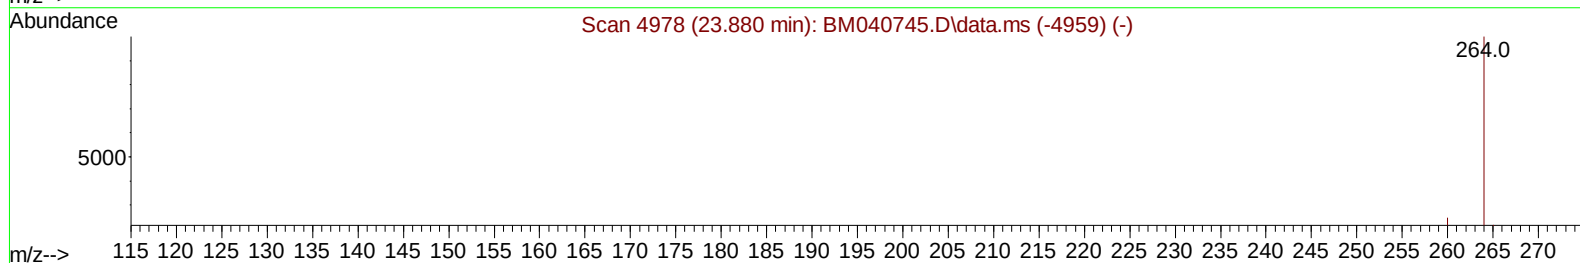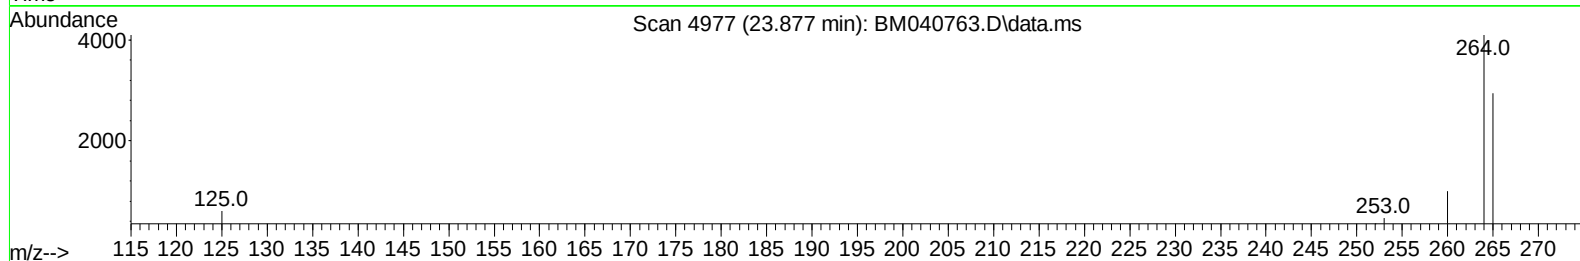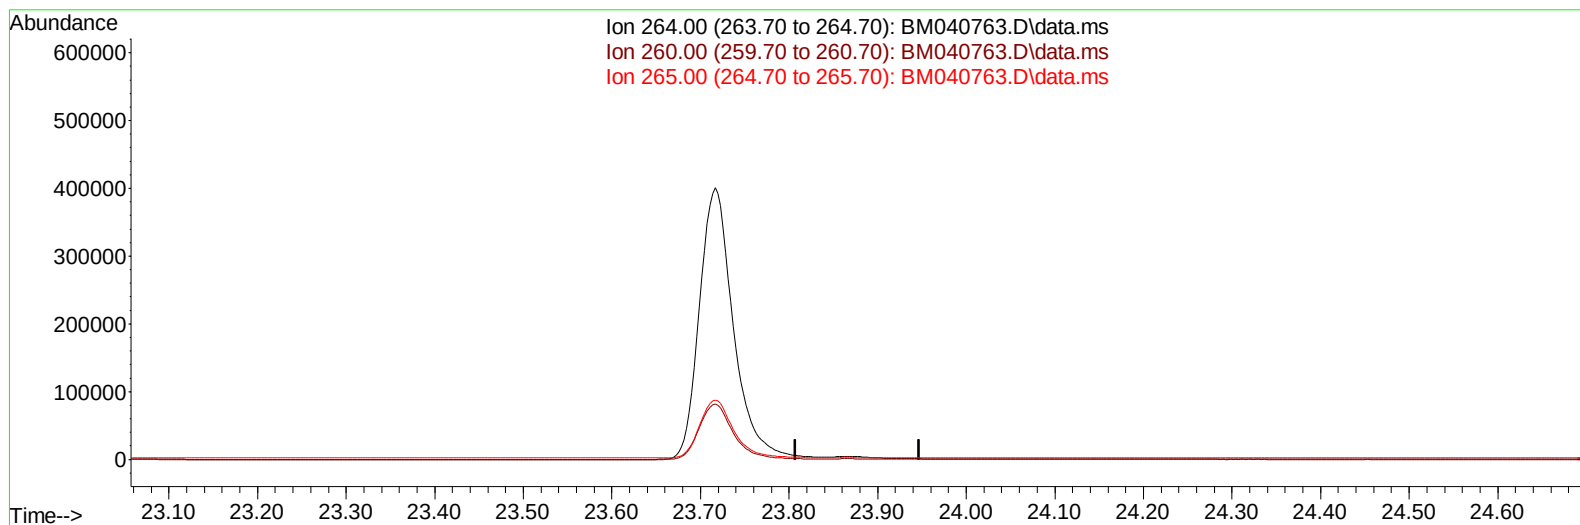

TIC: BM040763.D\data.ms

(23) Perylene-d12 (I)

23.877min (-23.877) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040763.D
 Acq On : 09 Jul 2023 06:25
 Operator : MA/JU
 Sample : PB153845BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK845

Manual IntegrationsAPPROVED

Quant Time: Jul 09 14:08:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

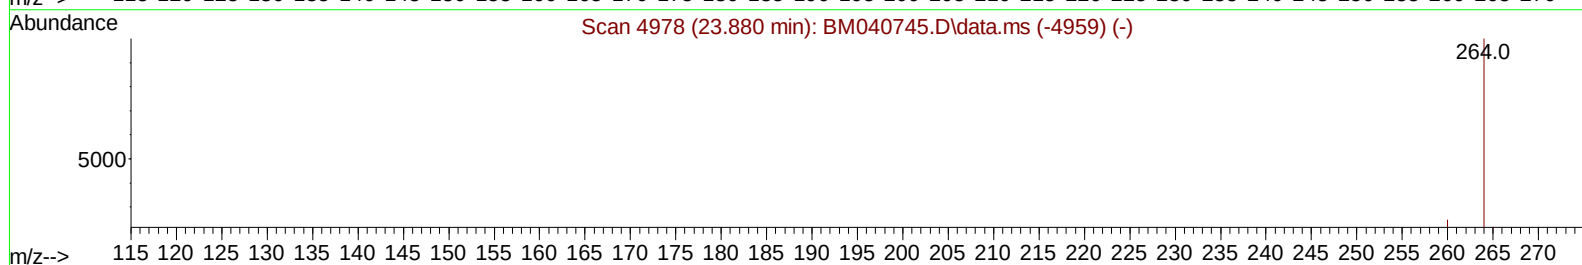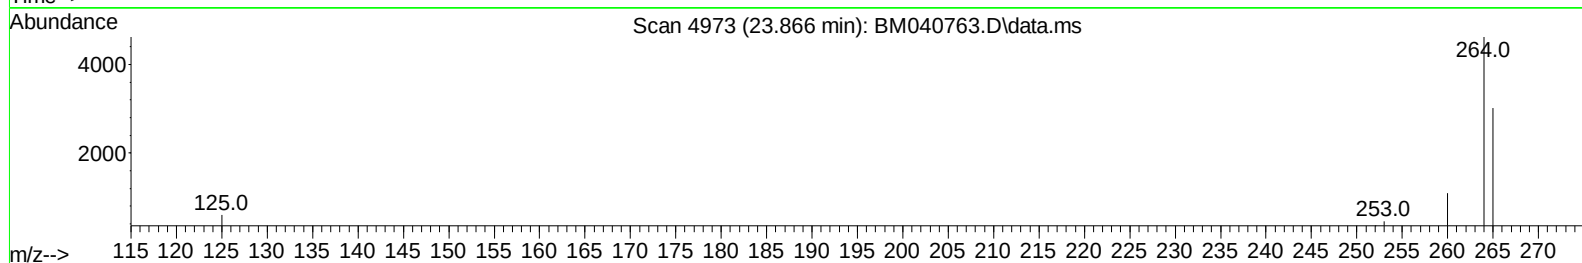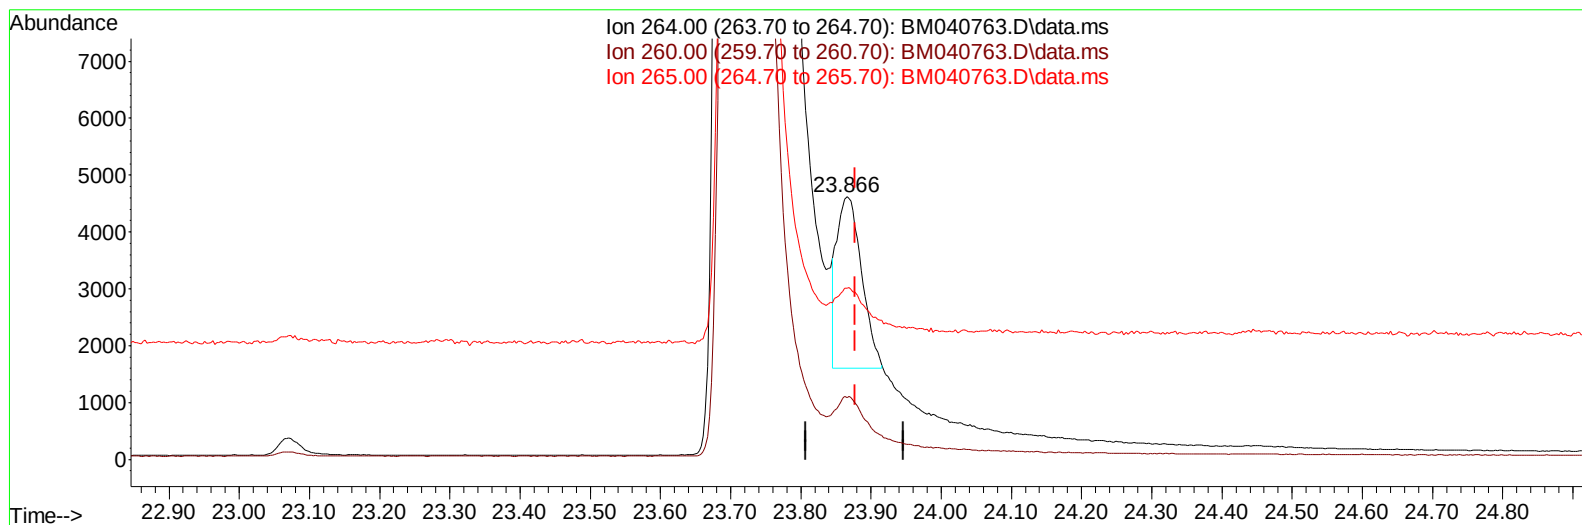

TIC: BM040763.D\data.ms

(23) Perylene-d12 (I)

23.866min (-0.012) 0.40 ng/ul m

response 7407

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.60
265.00	79.20	65.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040763.D
 Acq On : 09 Jul 2023 06:25
 Operator : MA/JU
 Sample : PB153845BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK845

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

Quant Time: Jul 09 14:08:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.891	152	3757	0.400	ng/ul	0.00
4) Naphthalene-d8	10.691	136	14101	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.532	164	7669	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.282	188	14207	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	8328	0.400	ng/ul	0.00
23) Perylene-d12	23.866	264	7407m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	16432	2.784	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	6038	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.315	212	13322	0.499	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040763.D
Acq On : 09 Jul 2023 06:25
Operator : MA/JU
Sample : PB153845BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK845

Manual IntegrationsAPPROVED

Quant Time: Jul 09 14:08:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 14:07:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

