




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040785.D
 Acq On : 09 Jul 2023 20:43
 Operator : MA/JU
 Sample : 03384-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 YBW82

Manual Integrations APPROVED

Reviewed By : Yogesh Patel 07/10/2023
 Supervised By : mohammad ahmed 07/10/2023

Quant Time: Jul 10 00:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

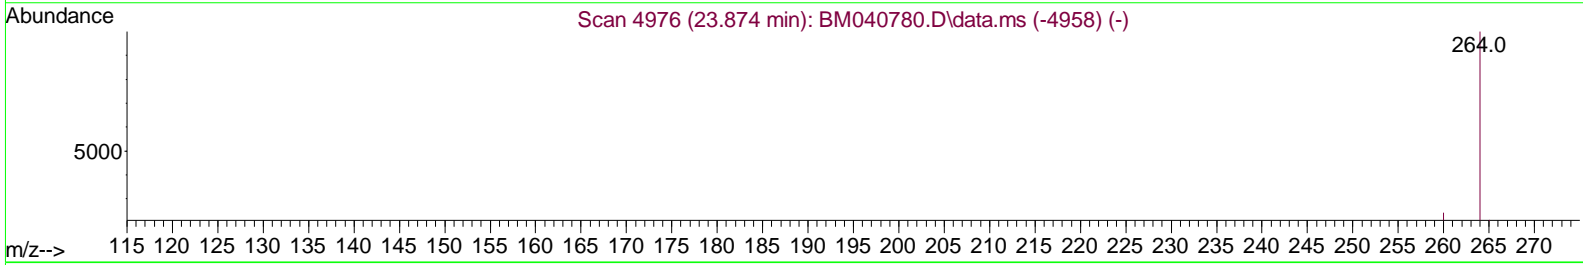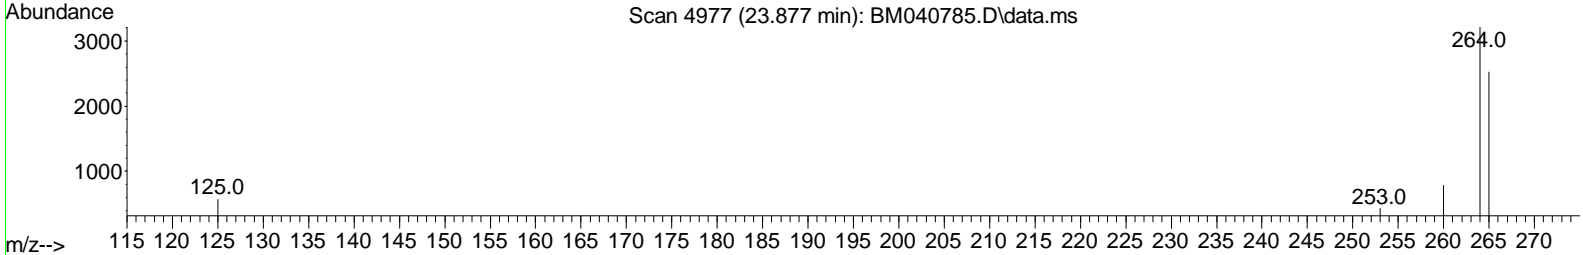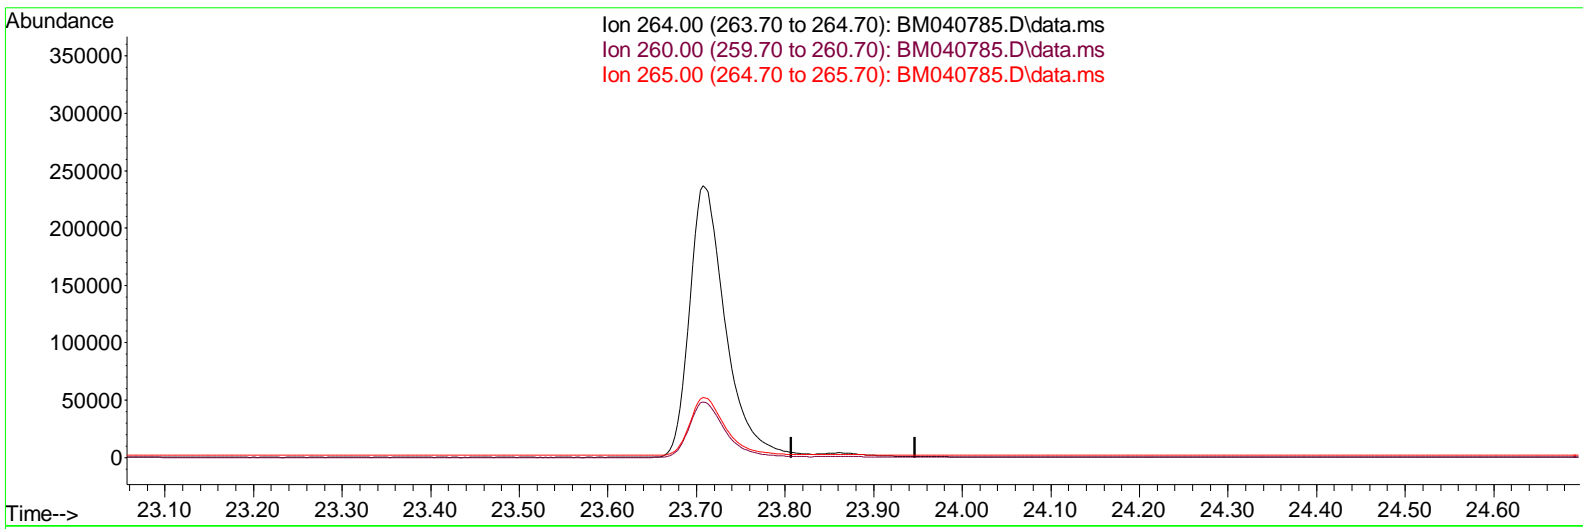

TIC: BM040785.D\data.ms

(23) Perylene-d12 (I)

23.877min (-23.877) 0.00 ng/ul

response 0

| Ion | Exp% | Act% |
|--------|--------|-------|
| 264.00 | 100.00 | 0.00 |
| 260.00 | 25.70 | 0.00# |
| 265.00 | 79.20 | 0.00# |
| 0.00 | 0.00 | 0.00 |




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040785.D
 Acq On : 09 Jul 2023 20:43
 Operator : MA/JU
 Sample : 03384-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBW82

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

Quant Time: Jul 10 00:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

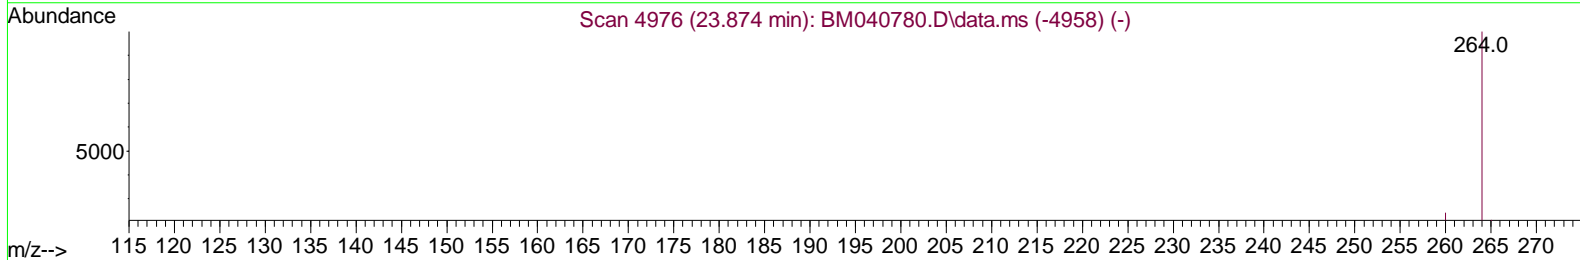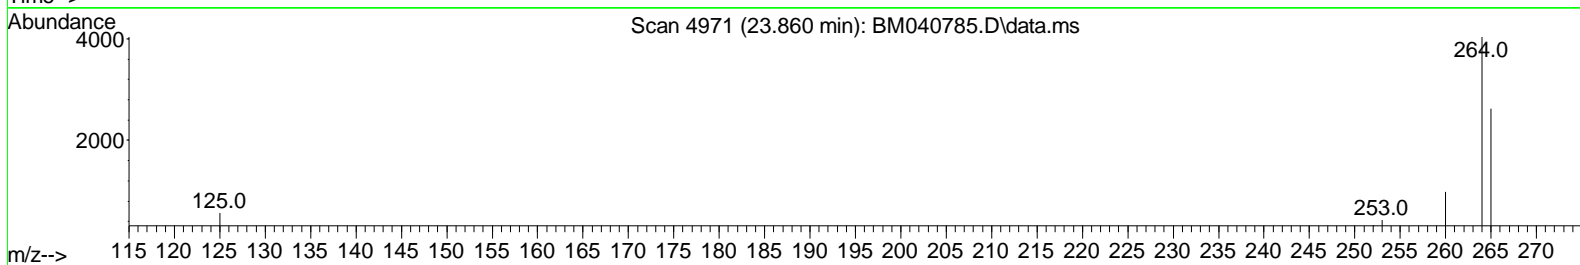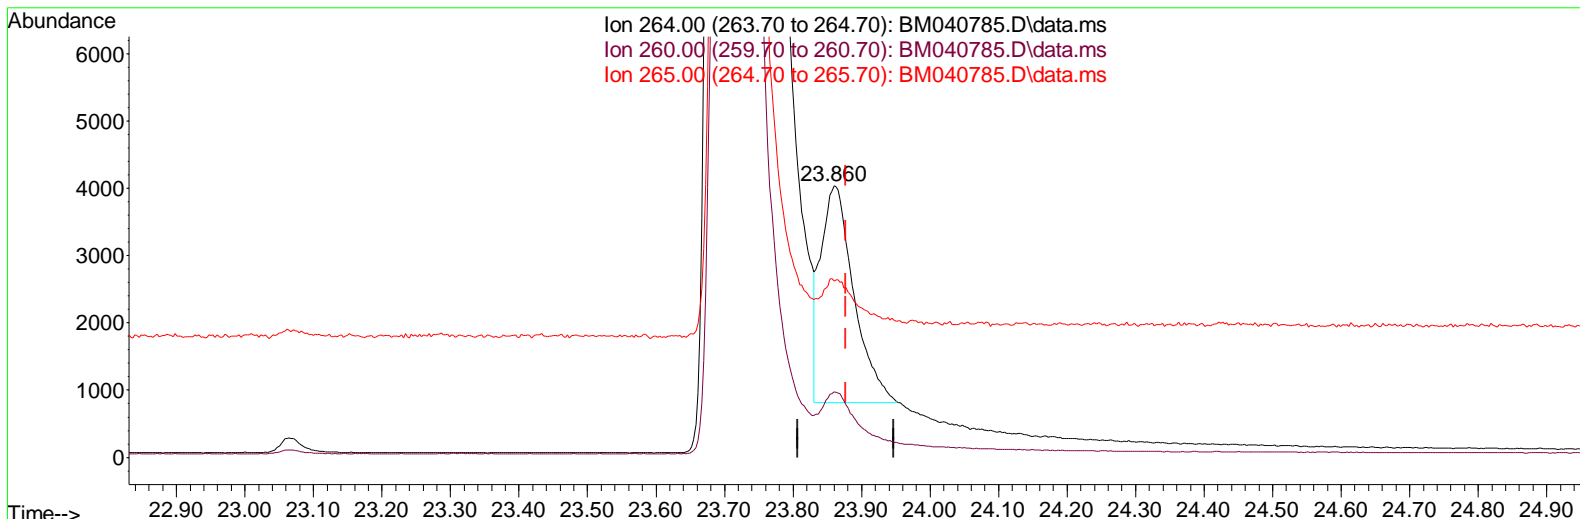

TIC: BM040785.D\data.ms

(23) Perylene-d12 (I)

23.860min (-0.017) 0.40 ng/ul m

| response | 10798 |
|----------|---------------|
| Ion | Exp% Act% |
| 264.00 | 100.00 100.00 |
| 260.00 | 25.70 24.26 |
| 265.00 | 79.20 65.04 |
| 0.00 | 0.00 0.00 |

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BMO70823\
 Data File : BMO40785.D
 Acq On : 09 Jul 2023 20:43
 Operator : MA/JU
 Sample : 03384-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 YBW82

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

Quant Time: Jul 10 00:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BMO62223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

| Compound | R.T. | QI on | Response | Conc | Units | Dev(Min) |
|------------------------------------|--------|-------|----------|-------|-------|----------|
| Internal Standards | | | | | | |
| 1) 1,4-Dichlorobenzene-d4 | 7.887 | 152 | 4152 | 0.400 | ng/ul | 0.00 |
| 4) Naphthalene-d8 | 10.686 | 136 | 15588 | 0.400 | ng/ul | #-0.01 |
| 9) Acenaphthene-d10 | 14.532 | 164 | 7903 | 0.400 | ng/ul | # 0.00 |
| 13) Phenanthrene-d10 | 17.282 | 188 | 13523 | 0.400 | ng/ul | -0.01 |
| 17) Chrysene-d12 | 21.475 | 240 | 8059 | 0.400 | ng/ul | 0.00 |
| 23) Perylene-d12 | 23.860 | 264 | 10798m | 0.400 | ng/ul | -0.02 |
| System Monitoring Compounds | | | | | | |
| 3) 1,4-Dioxane-d8 | 3.296 | 96 | 12599 | 1.932 | ng/ul | 0.00 |
| 6) 2-Methylnaphthalene-d10 | 12.280 | 152 | 5275 | 0.241 | ng/ul | -0.01 |
| 18) Fluoranthene-d10 | 19.311 | 212 | 7953 | 0.308 | ng/ul | -0.01 |

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040785.D
 Acq On : 09 Jul 2023 20:43
 Operator : MA/JU
 Sample : 03384-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 YBW82

Manual Integrations APPROVED

Reviewed By : Yogesh Patel 07/10/2023
 Supervised By : mohammad ahmed 07/10/2023

Quant Time: Jul 10 00:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

