

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040736.D
 Acq On : 08 Jul 2023 12:14
 Operator : MA/JU
 Sample : 03332-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBTY8

Quant Time: Jul 08 22:57:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 22:50:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	3916	0.400	ng/ul	0.00
4) Naphthalene-d8	10.696	136	14654	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.536	164	7971	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.286	188	15812	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	10906	0.400	ng/ul	0.00
23) Perylene-d12	23.874	264	10501	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	32711	5.318	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	7227	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	12531	0.358	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.338	88	1355	0.216	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040736.D
Acq On : 08 Jul 2023 12:14
Operator : MA/JU
Sample : 03332-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBTY8

Quant Time: Jul 08 22:57:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 22:50:20 2023
Response via : Initial Calibration

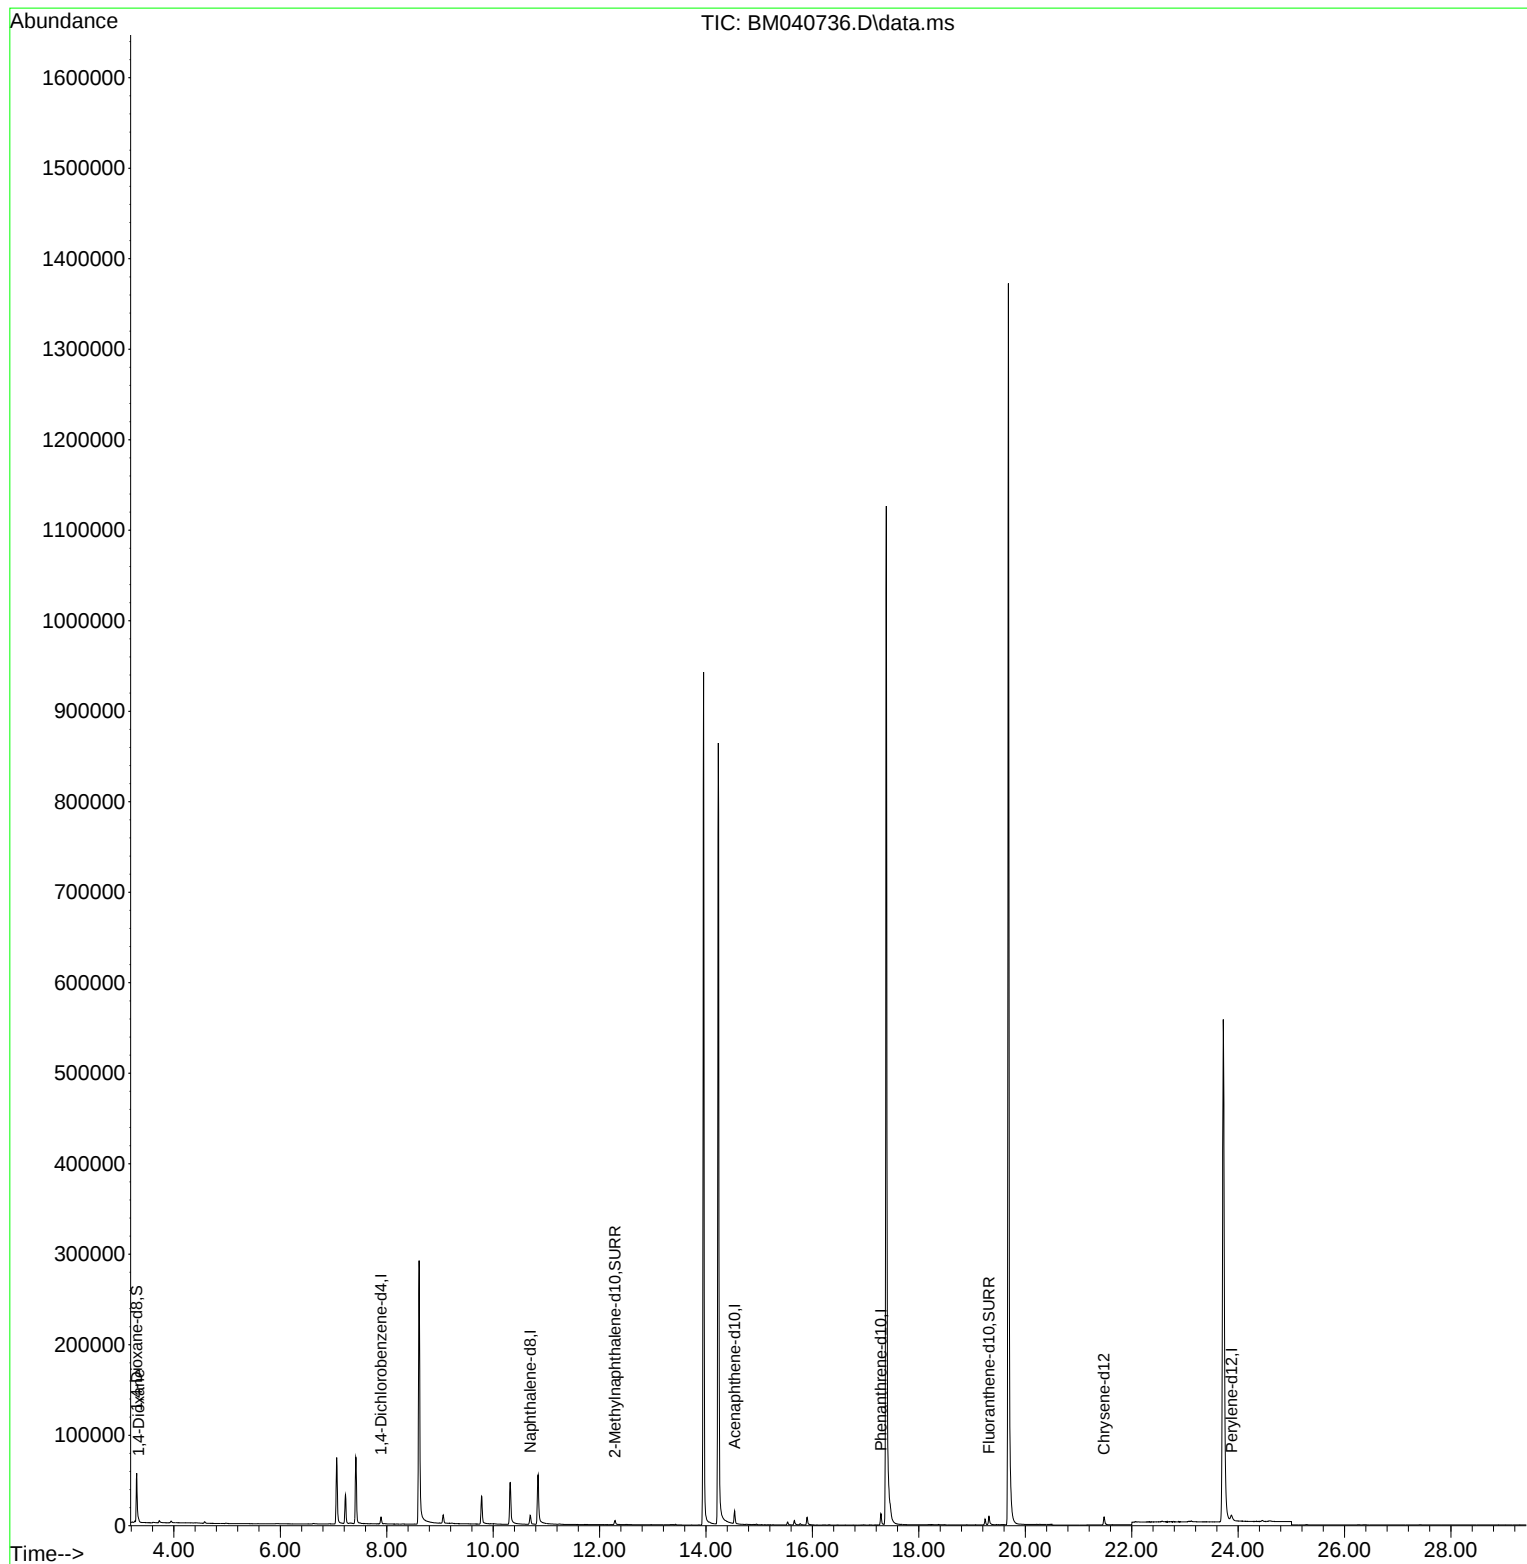

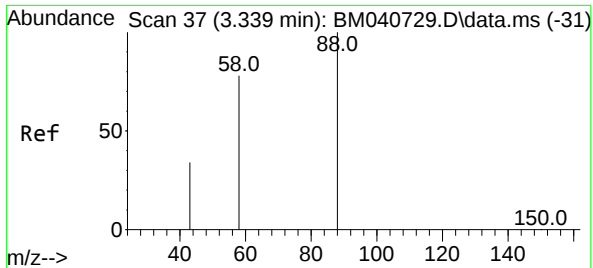

#2
 1,4-Dioxane
 Concen: 0.216 ng/ul
 RT: 3.338 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM040736.D
 Acq: 08 Jul 2023 12:14

Instrument :
 BNA_M
 ClientSampleId :
 YBTY8

Tgt Ion: 88 Resp: 1355

Ion	Ratio	Lower	Upper
88	100		
43	84.3	36.1	54.1#
58	63.1	49.8	74.8

