

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
 Data File : BM040772.D
 Acq On : 09 Jul 2023 12:01
 Operator : MA/JU
 Sample : 03356-09
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBW38

Quant Time: Jul 09 14:41:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 14:07:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	4114	0.400	ng/ul	0.00
4) Naphthalene-d8	10.691	136	14812	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.532	164	7689	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.282	188	14415	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	9659	0.400	ng/ul	0.00
23) Perylene-d12	23.865	264	9105	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	35062	5.426	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	7388	0.356	ng/ul	-0.01
18) Fluoranthene-d10	19.315	212	11606	0.375	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.334	88	1506	0.229	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070823\
Data File : BM040772.D
Acq On : 09 Jul 2023 12:01
Operator : MA/JU
Sample : 03356-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBW38

Quant Time: Jul 09 14:41:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 14:07:58 2023
Response via : Initial Calibration

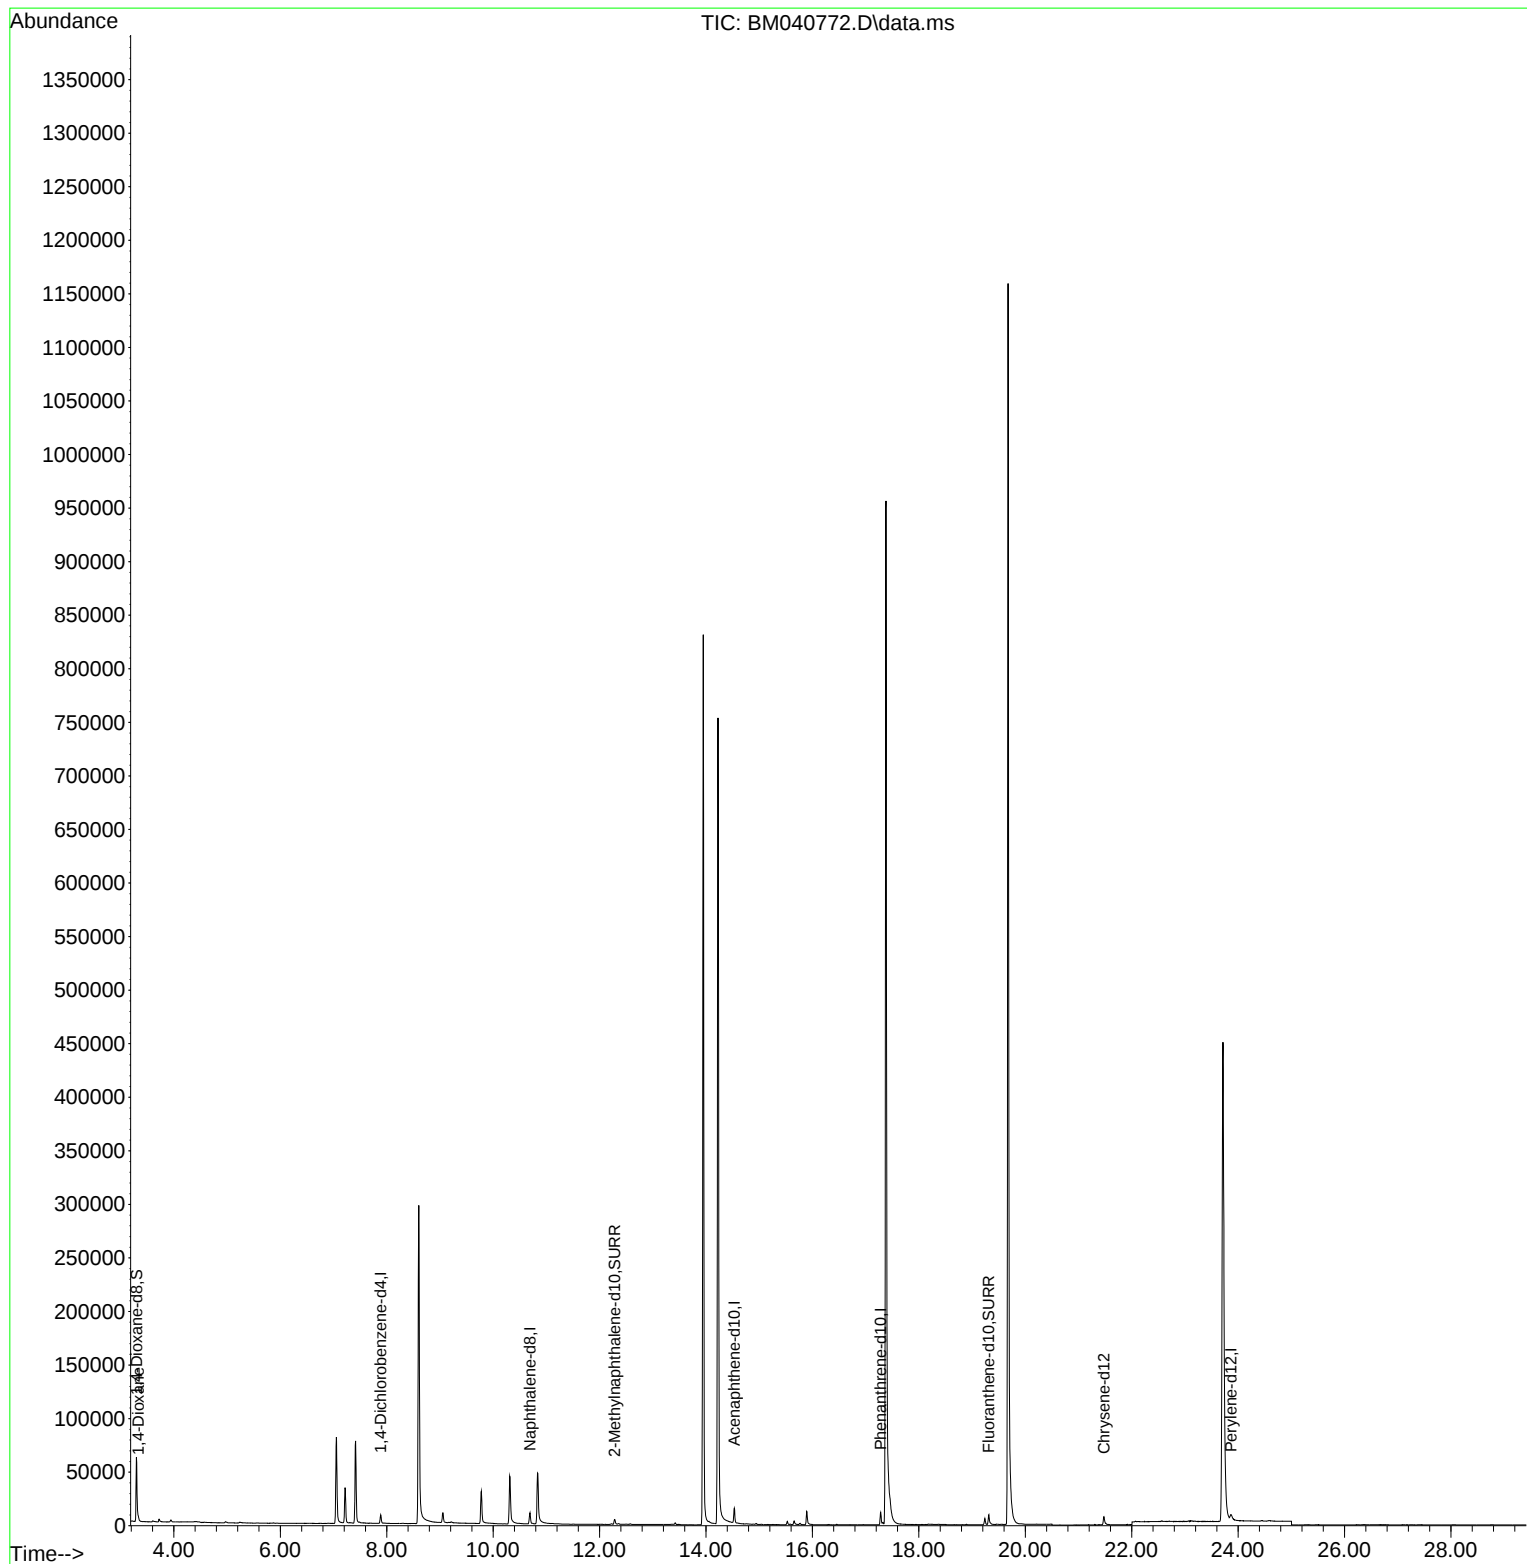

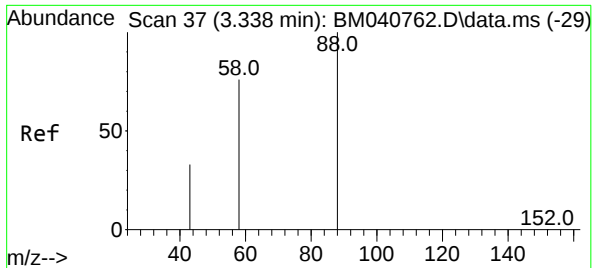

#2
 1,4-Dioxane
 Concen: 0.229 ng/ul
 RT: 3.334 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM040772.D
 Acq: 09 Jul 2023 12:01

Instrument :
 BNA_M
 ClientSampleId :
 YBW38

Tgt Ion: 88 Resp: 1506

Ion	Ratio	Lower	Upper
88	100		
43	88.0	36.1	54.1#
58	61.2	49.8	74.8

