


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070918\
 Data File : BM015838.D
 Acq On : 09 Jul 2018 11:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

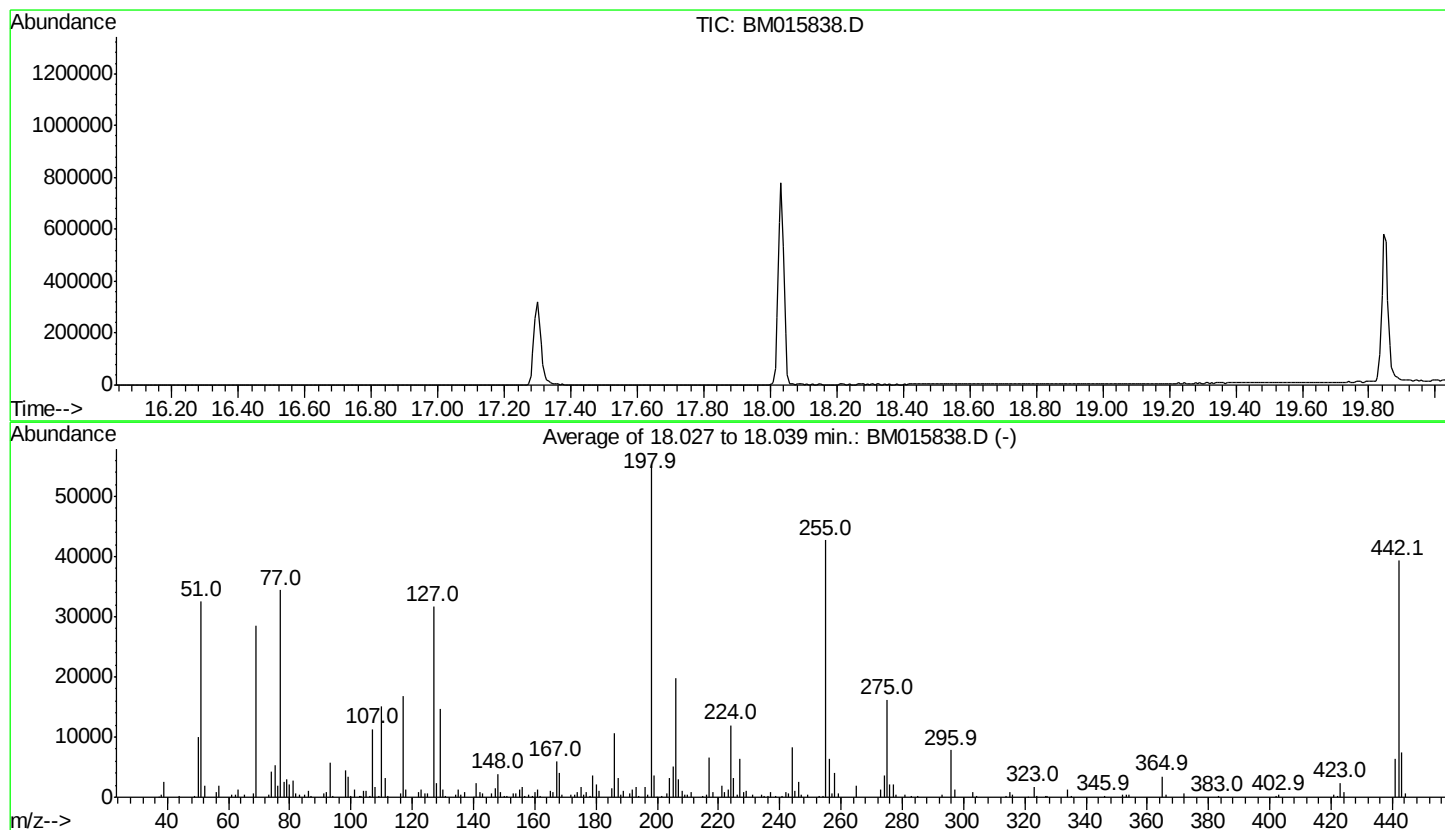

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.0	32488	PASS
68	69	0.00	2	1.9	545	PASS
69	198	0.00	100	51.6	28426	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.4	31616	PASS
197	198	0.00	2	0.8	436	PASS
198	198	100	100	100.0	55090	PASS
199	198	5	9	6.6	3654	PASS
275	198	10	60	29.3	16166	PASS
365	198	1	100	6.4	3503	PASS
441	443	0.01	100	85.6	6381	PASS
442	198	50	100	71.3	39264	PASS
443	442	15	24	19.0	7458	PASS