


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070918\
 Data File : BM015857.D
 Acq On : 10 Jul 2018 00:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

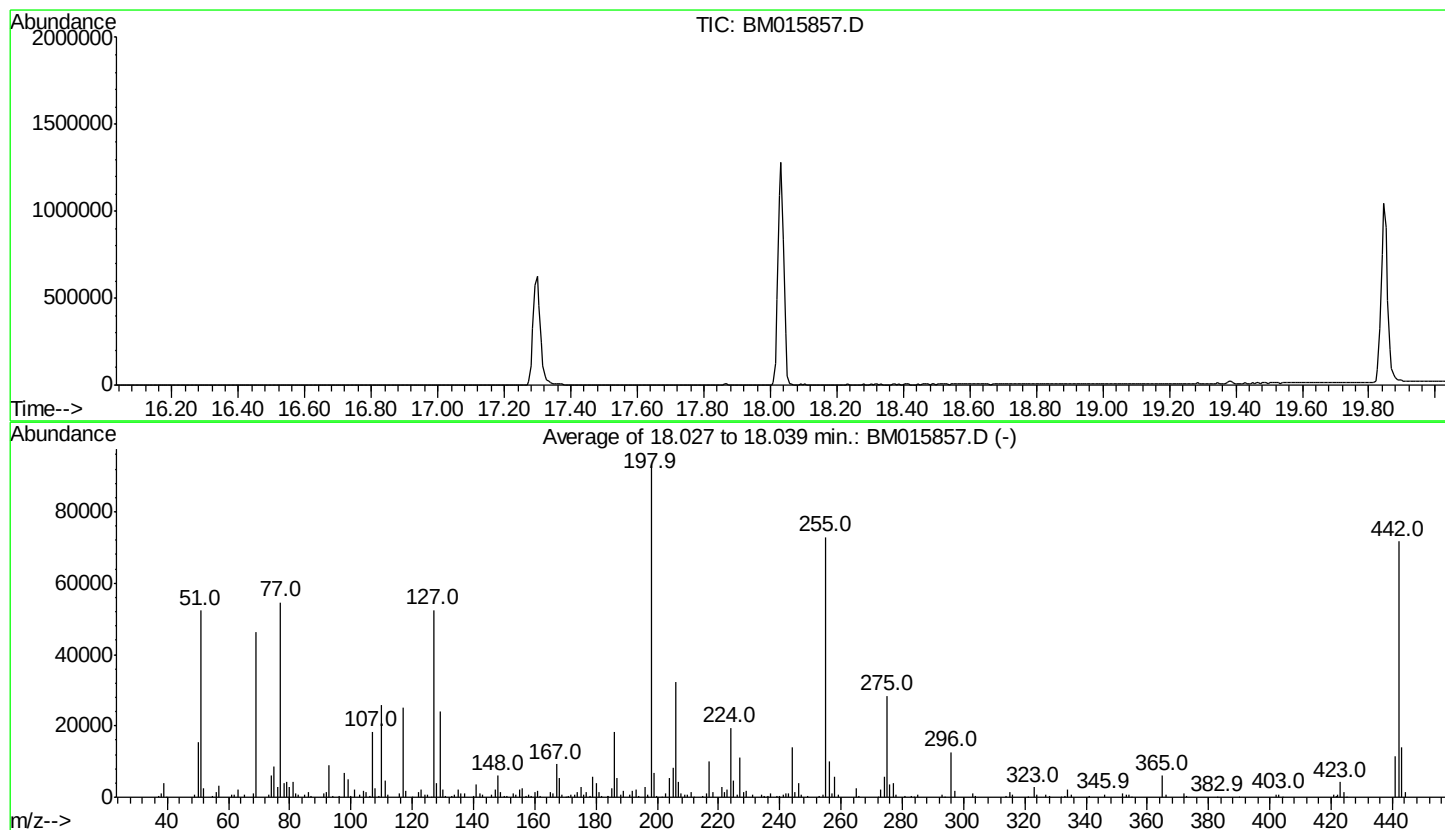

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	52317	PASS
68	69	0.00	2	2.0	913	PASS
69	198	0.00	100	49.6	46114	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.4	52389	PASS
197	198	0.00	2	0.7	672	PASS
198	198	100	100	100.0	92933	PASS
199	198	5	9	7.4	6908	PASS
275	198	10	60	30.6	28408	PASS
365	198	1	100	6.4	5944	PASS
441	443	0.01	100	81.4	11500	PASS
442	198	50	100	77.2	71733	PASS
443	442	15	24	19.7	14121	PASS