

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM070920\  
 Data File : BM026699.D  
 Acq On : 08 Jul 2020 09:36  
 Operator : JU/CG  
 Sample : PB129955BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB129955BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM070820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.963       | 347           | 353         | 372          | rBV      | 1555357        | 2256289       | 27.79%          | 7.239%        |
| 2         | 6.534       | 611           | 620         | 638          | rBV      | 1645299        | 2505794       | 30.87%          | 8.040%        |
| 3         | 7.328       | 747           | 755         | 765          | rBV      | 287559         | 451296        | 5.56%           | 1.448%        |
| 4         | 7.640       | 801           | 808         | 821          | rBV      | 1292047        | 1997236       | 24.60%          | 6.408%        |
| 5         | 8.475       | 943           | 950         | 978          | rBV      | 1169517        | 1891210       | 23.30%          | 6.068%        |
| 6         | 10.081      | 1216          | 1223        | 1240         | rBV      | 376038         | 659535        | 8.12%           | 2.116%        |
| 7         | 12.592      | 1643          | 1650        | 1670         | rBV      | 2852333        | 4217832       | 51.95%          | 13.533%       |
| 8         | 13.986      | 1881          | 1887        | 1898         | rBV2     | 653770         | 955368        | 11.77%          | 3.065%        |
| 9         | 15.498      | 2137          | 2144        | 2165         | rBV      | 2758864        | 3757225       | 46.28%          | 12.055%       |
| 10        | 16.745      | 2350          | 2356        | 2373         | rBV      | 813804         | 1190330       | 14.66%          | 3.819%        |
| 11        | 19.410      | 2803          | 2809        | 2814         | rBV      | 6698279        | 8118455       | 100.00%         | 26.047%       |
| 12        | 20.962      | 3068          | 3073        | 3084         | rBV      | 1142816        | 1549156       | 19.08%          | 4.970%        |
| 13        | 23.039      | 3420          | 3426        | 3438         | rVB      | 934985         | 1618418       | 19.94%          | 5.193%        |


Sum of corrected areas: 31168144

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070920\  
Data File : BM026699.D  
Acq On : 08 Jul 2020 09:36  
Operator : JU/CG  
Sample : PB129955BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB129955BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

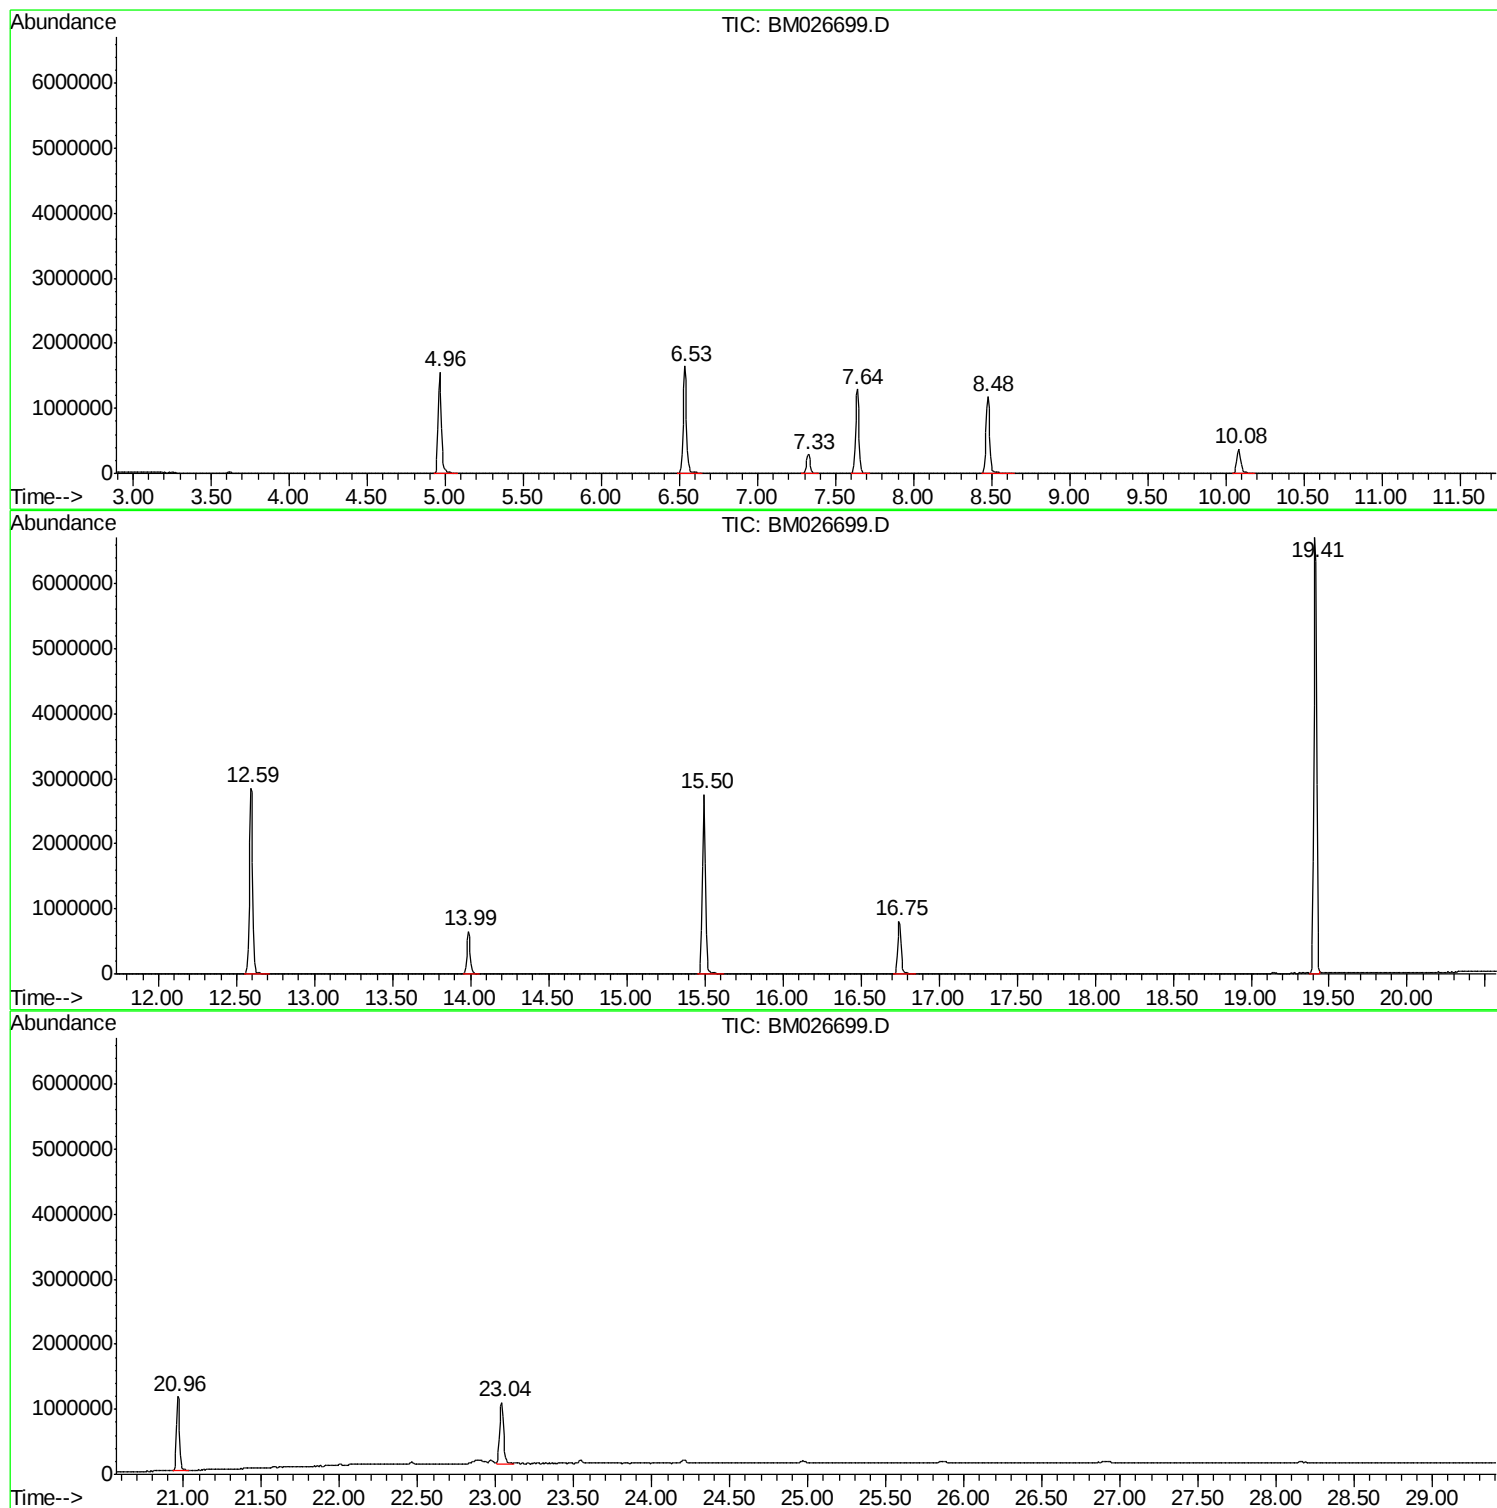

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM070920\  
Data File : BM026699.D  
Acq On : 08 Jul 2020 09:36  
Operator : JU/CG  
Sample : PB129955BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB129955BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM070820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM070920\  
Data File : BM026699.D  
Acq On : 08 Jul 2020 09:36  
Operator : JU/CG  
Sample : PB129955BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB129955BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM070820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |