


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070920\
 Data File : BM026697.D
 Acq On : 08 Jul 2020 08:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 08 11:38:47 2020

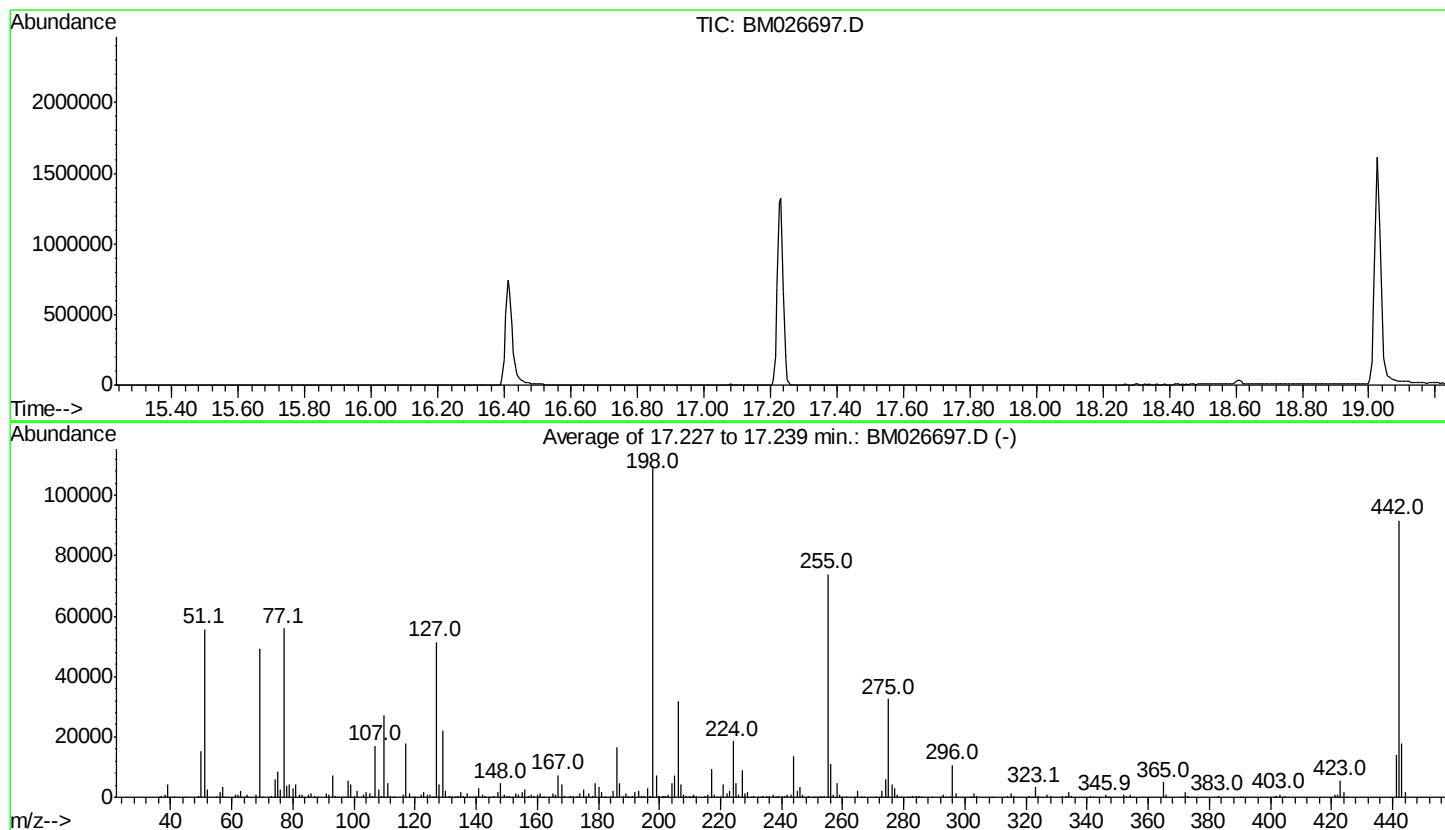

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	55685	PASS
68	69	0.00	2	1.9	915	PASS
69	198	0.00	100	44.9	49394	PASS
70	69	0.00	2	0.4	206	PASS
127	198	10	80	46.8	51421	PASS
197	198	0.00	2	0.5	528	PASS
198	198	100	100	100.0	109904	PASS
199	198	5	9	6.8	7428	PASS
275	198	10	60	29.7	32653	PASS
365	198	1	100	4.6	5072	PASS
441	198	0.01	100	12.8	14089	PASS
442	198	50	100	83.4	91640	PASS
443	442	15	24	19.3	17725	PASS