

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071018\
 Data File : BM015882.D
 Acq On : 10 Jul 2018 23:53
 Operator : SJ/JU
 Sample : PB110959BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB110959BL

Quant Time: Jul 11 03:48:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 05 17:39:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	68195	20.00	ng	-0.02
21) Naphthalene-d8	11.13	136	279381	20.00	ng	-0.02
38) Acenaphthene-d10	14.92	164	175315	20.00	ng	-0.02
63) Phenanthrene-d10	17.64	188	414841	20.00	ng	-0.01
75) Chrysene-d12	21.75	240	405574	20.00	ng	-0.02
86) Perylene-d12	24.15	264	372028	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	707538	177.93	ng	-0.02
7) Phenol-d6	7.45	99	962469	176.80	ng	-0.01
23) Nitrobenzene-d5	9.49	82	613296	107.11	ng	-0.02
41) 2,4,6-Tribromophenol	16.40	330	414389	180.90	ng	-0.02
44) 2-Fluorobiphenyl	13.54	172	1454224	102.98	ng	-0.02
78) Terphenyl-d14	20.21	244	2795322	127.84	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071018\
Data File : BM015882.D
Acq On : 10 Jul 2018 23:53
Operator : SJ/JU
Sample : PB110959BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110959BL

Quant Time: Jul 11 03:48:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

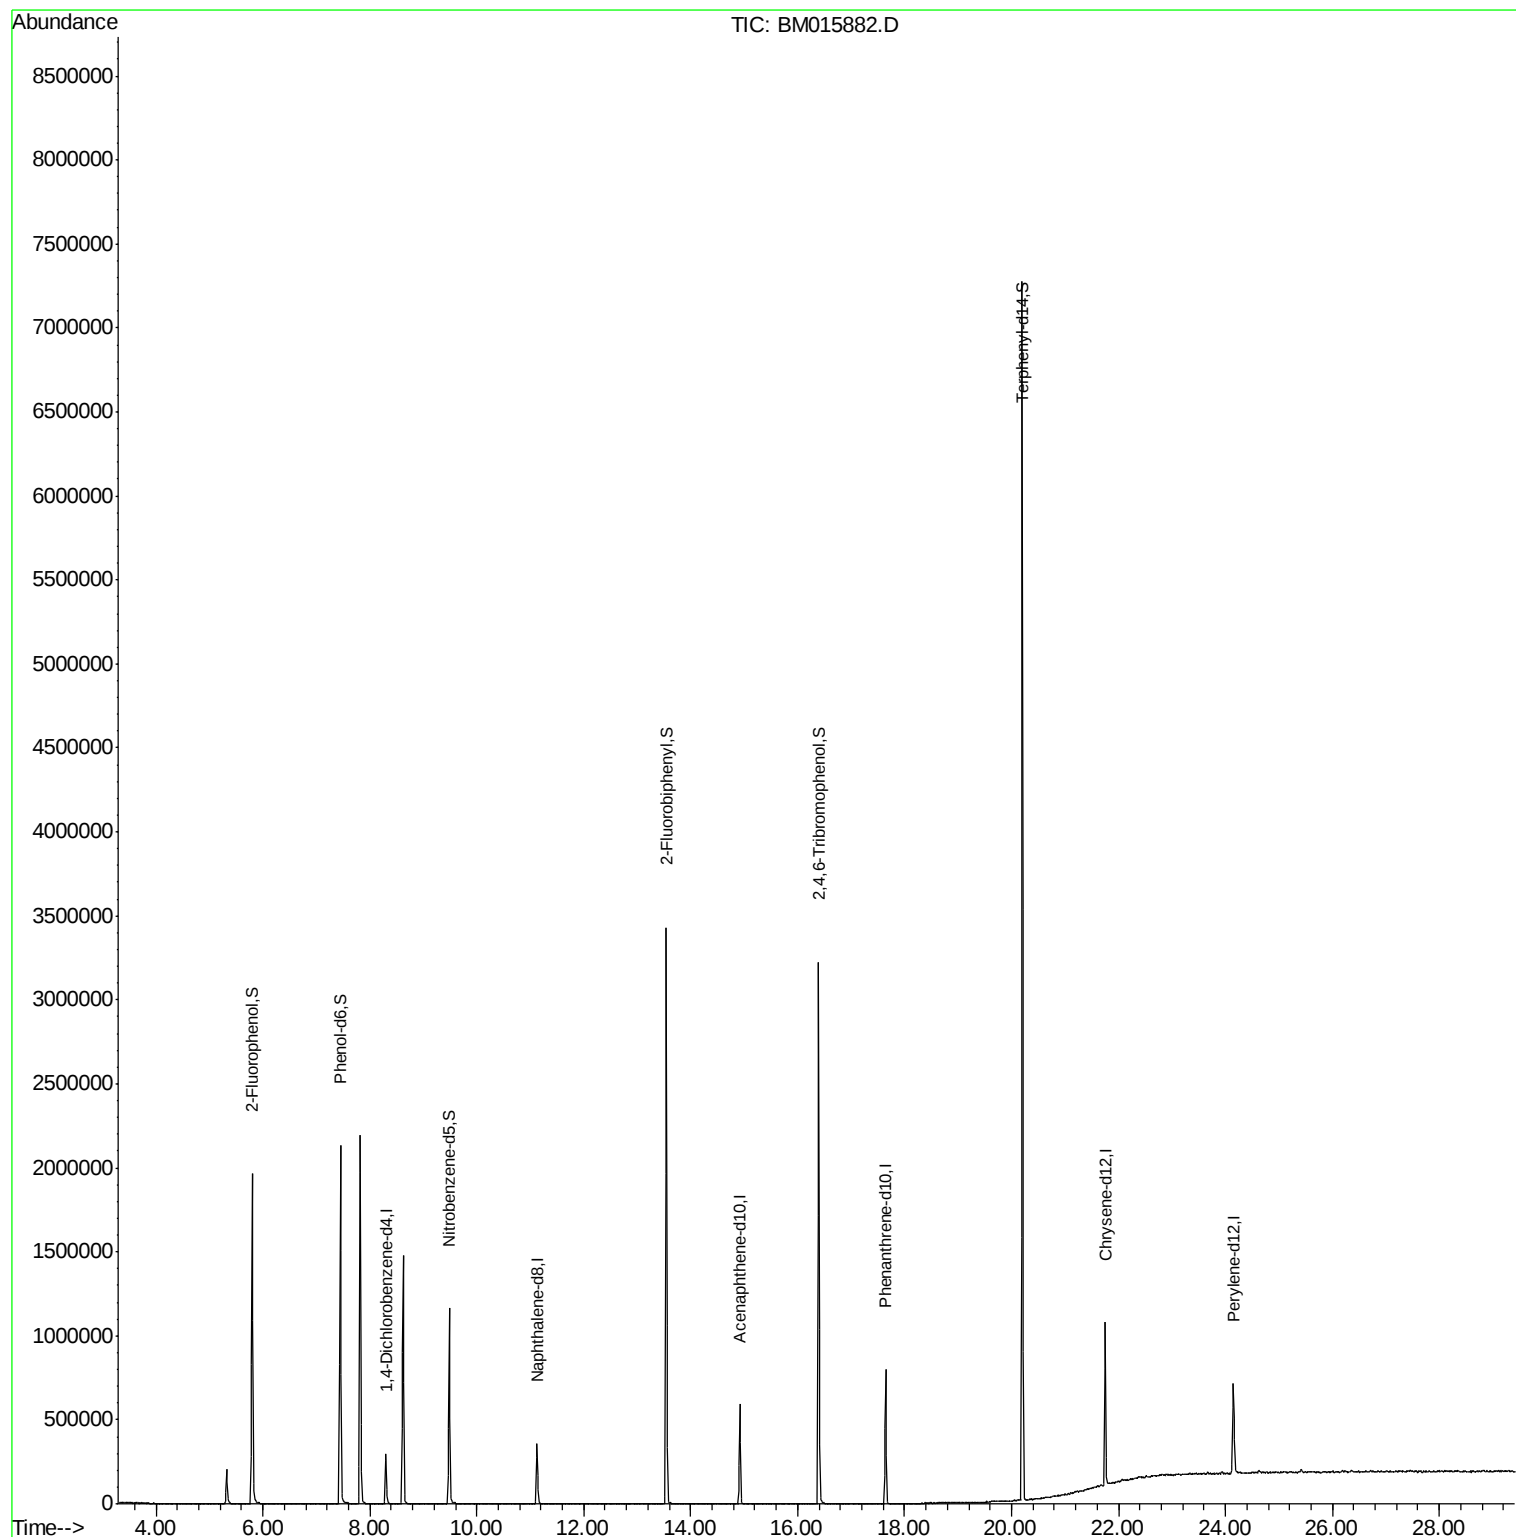




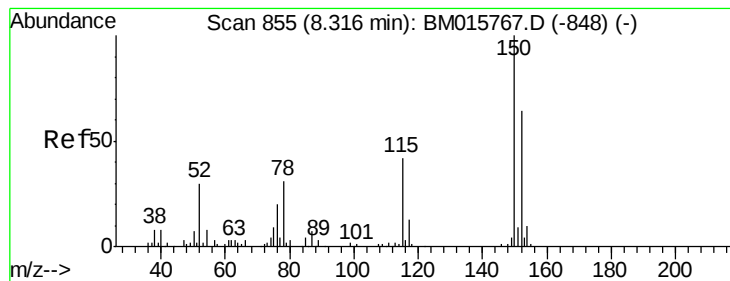


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.30 min Scan# 852
 Delta R.T. -0.02 min
 Lab File: BM015882.D
 Acq: 10 Jul 2018 23:53

Instrument :
 BNA_M
 ClientSampleId :
 PB110959BL




Tgt Ion:152 Resp: 68195
 Ion Ratio Lower Upper
 152 100
 150 151.0 119.5 179.3
 115 65.8 43.0 64.4#

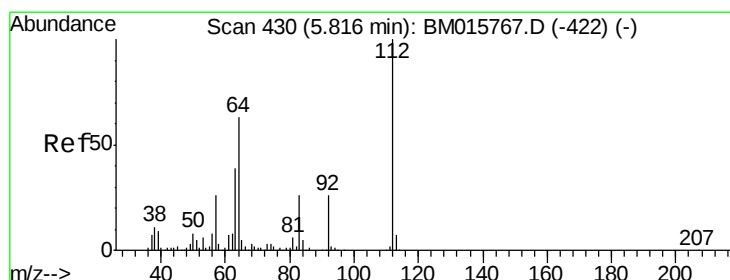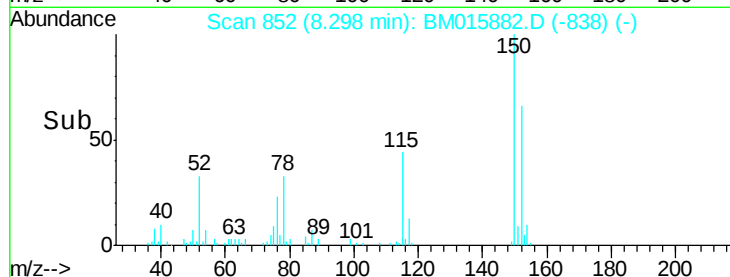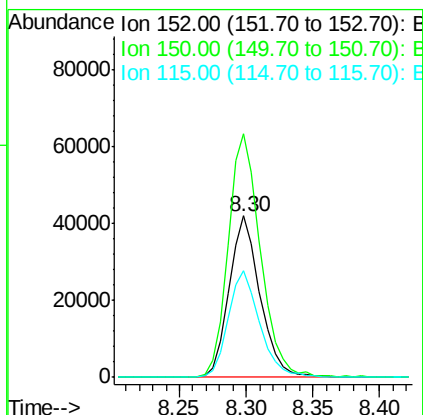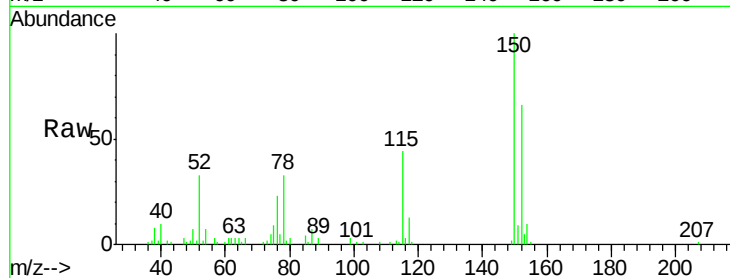


#5

2-Fluorophenol
 Concen: N.D. ng
 RT: 5.80 min Scan# 427
 Delta R.T. -0.02 min
 Lab File: BM015882.D
 Acq: 10 Jul 2018 23:53

Tgt Ion:112 Resp: 707538
 Ion Ratio Lower Upper
 112 100
 64 64.7 38.6 57.8#
 63 40.4 19.3 28.9#

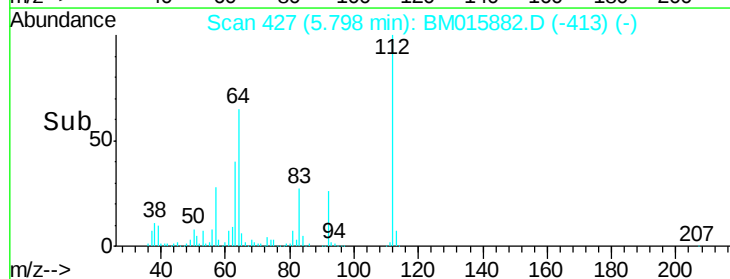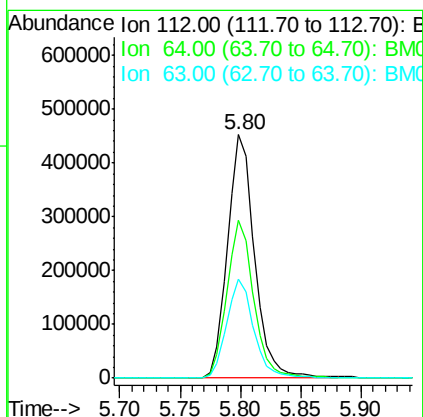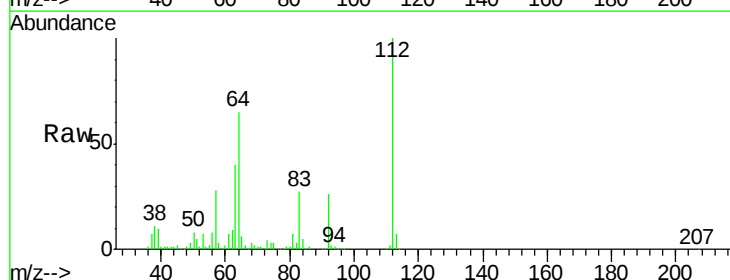

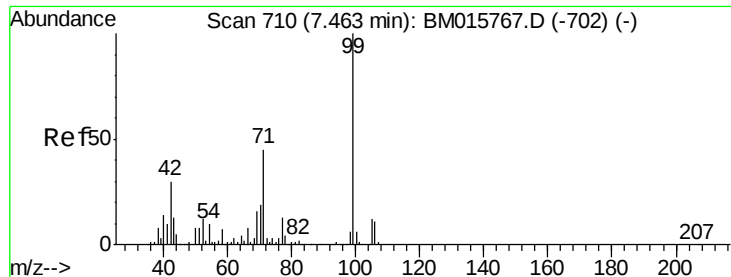

#7

Phenol-d6

Concen: N.D. ng

RT: 7.45 min Scan# 708

Delta R.T. -0.01 min

Lab File: BM015882.D

Acq: 10 Jul 2018 23:53

Instrument :

BNA_M

ClientSampleId :

PB110959BL


Tgt Ion: 99 Resp: 962469

Ion Ratio Lower Upper

99 100

42 31.0 11.0 16.4#




71 45.8 23.4 35.2#

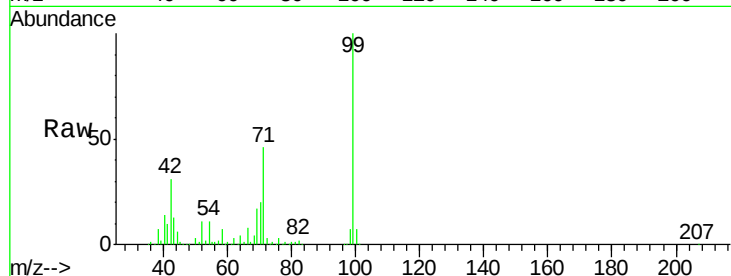

Abundance Ion 99.00 (98.70 to 99.70): BM015767.D (-702) (-)

Ion 42.00 (41.70 to 42.70): BM015767.D (-702) (-)

Ion 71.00 (70.70 to 71.70): BM015767.D (-702) (-)

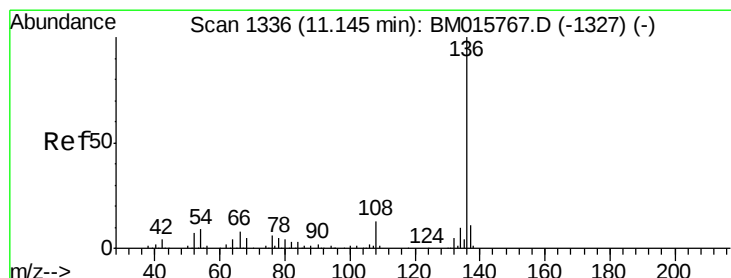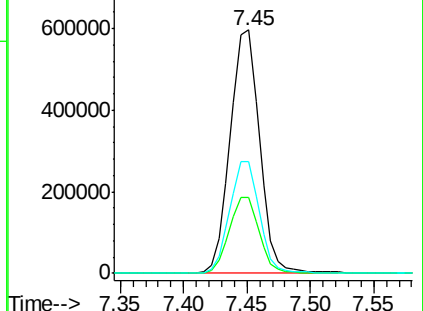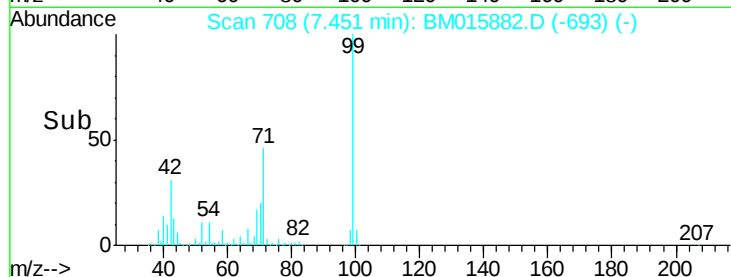

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.13 min Scan# 1333

Delta R.T. -0.02 min

Lab File: BM015882.D

Acq: 10 Jul 2018 23:53

Tgt Ion: 136 Resp: 279381


Ion Ratio Lower Upper

136 100

137 11.1 8.7 13.1

54 9.0 4.6 6.8#

68 4.2 3.7 5.5


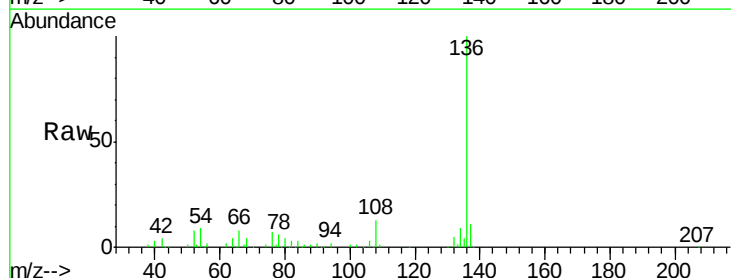



Abundance Ion 136.00 (135.70 to 136.70): BM015767.D (-1327) (-)

Ion 137.00 (136.70 to 137.70): BM015767.D (-1327) (-)

Ion 54.00 (53.70 to 54.70): BM015767.D (-1327) (-)

Ion 68.00 (67.70 to 68.70): BM015767.D (-1327) (-)



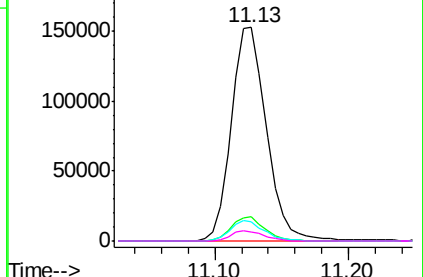
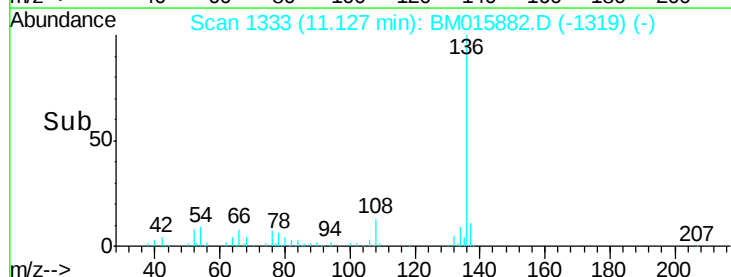


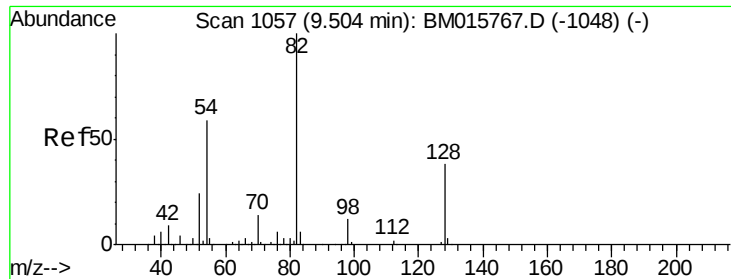

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.49 min Scan# 1054
Delta R.T. -0.02 min
Lab File: BM015882.D
Acq: 10 Jul 2018 23:53




Instrument :
BNA_M
ClientSampleId :
PB110959BL


Tgt Ion	Ratio	Lower	Upper
82	100		
128	38.3	32.8	49.2
54	60.8	40.6	60.8

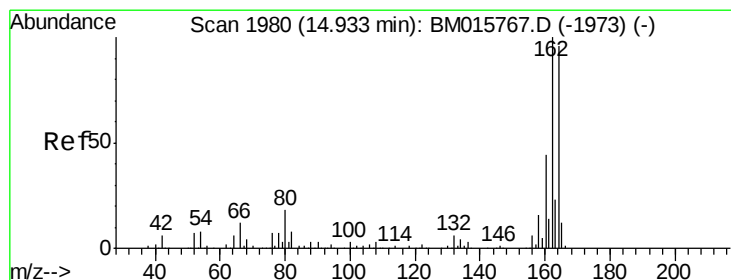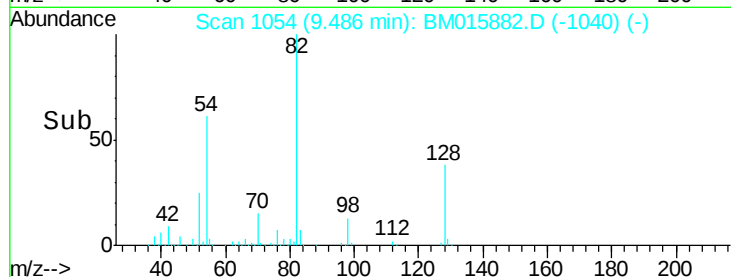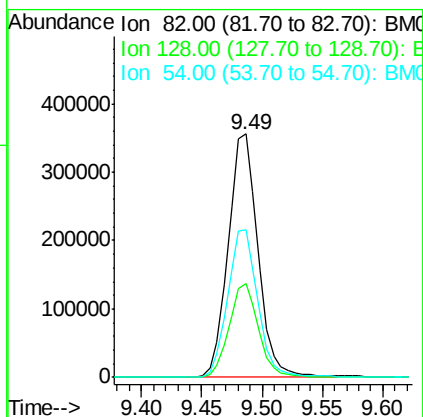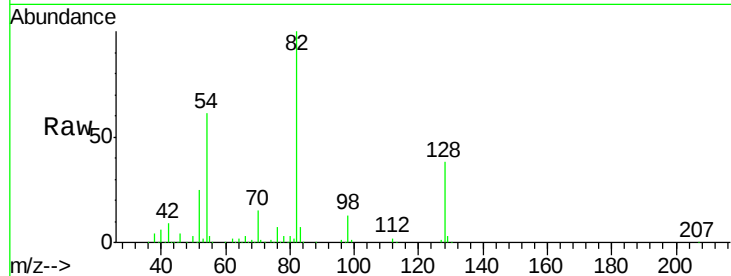

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.92 min Scan# 1977
Delta R.T. -0.02 min
Lab File: BM015882.D
Acq: 10 Jul 2018 23:53

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.1	82.4	123.6
160	47.9	35.8	53.6

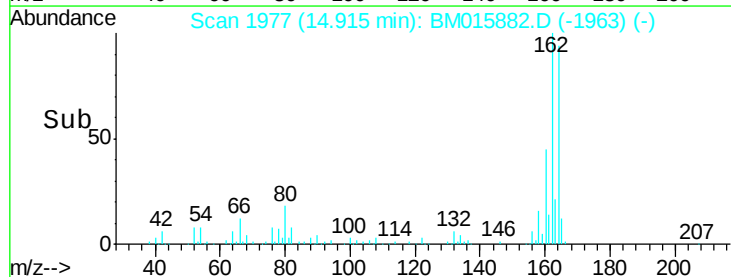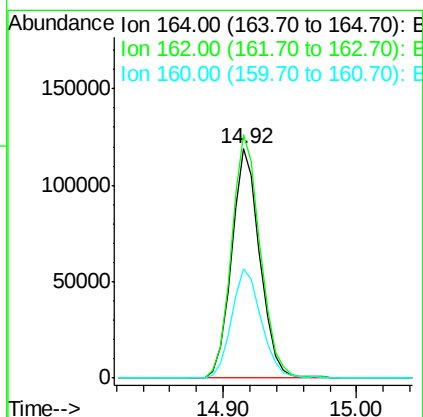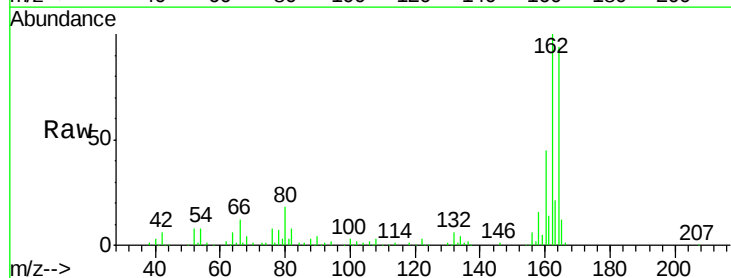


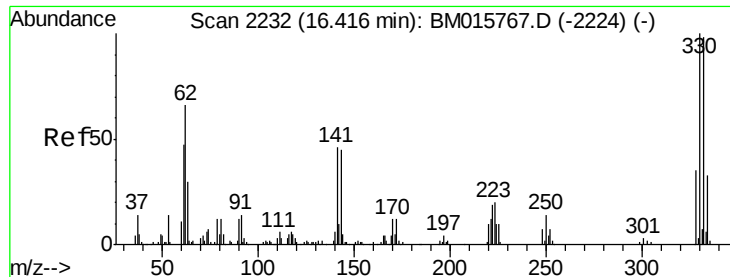




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.40 min Scan# 2229
 Delta R.T. -0.02 min
 Lab File: BM015882.D
 Acq: 10 Jul 2018 23:53

Instrument :
 BNA_M
 ClientSampleId :
 PB110959BL

Tgt Ion:330 Resp: 414389
 Ion Ratio Lower Upper
 330 100
 332 96.8 0.0 0.0#
 141 55.1 0.0 0.0#

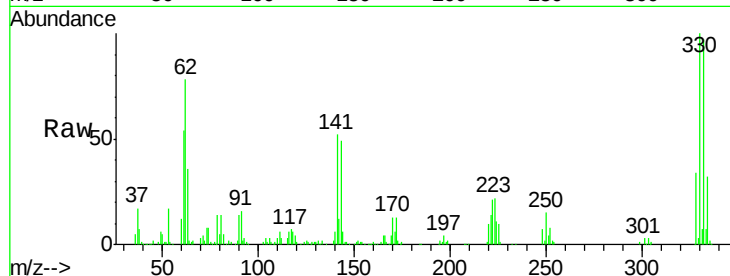


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

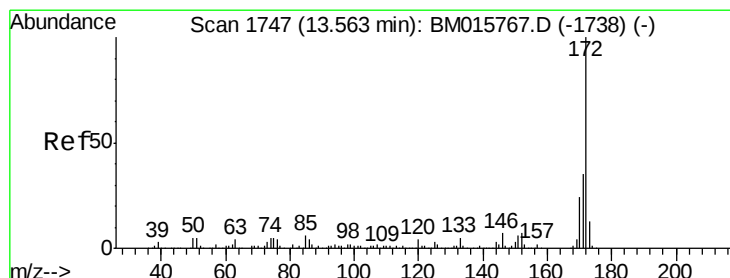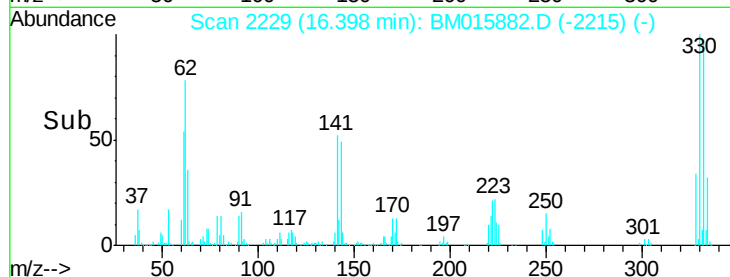
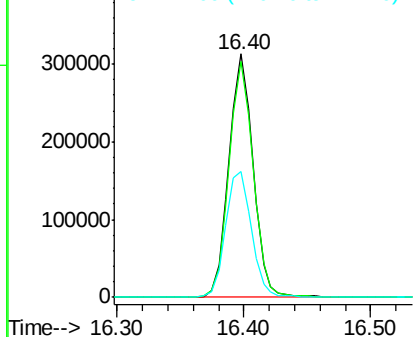



#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.54 min Scan# 1744
 Delta R.T. -0.02 min
 Lab File: BM015882.D
 Acq: 10 Jul 2018 23:53

Tgt Ion:172 Resp: 1454224
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.5 42.7
 170 23.8 18.8 28.2

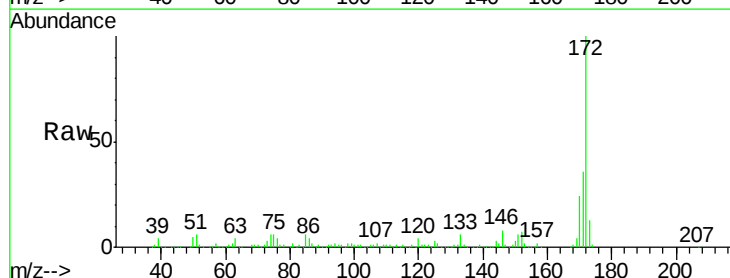

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



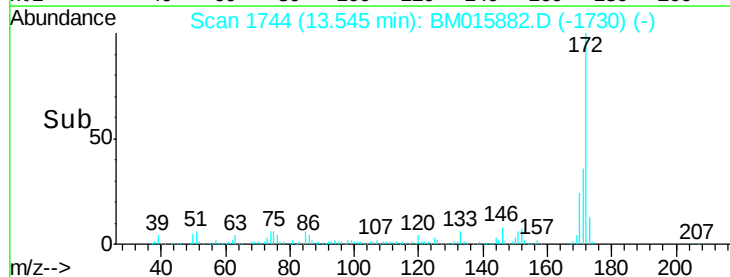
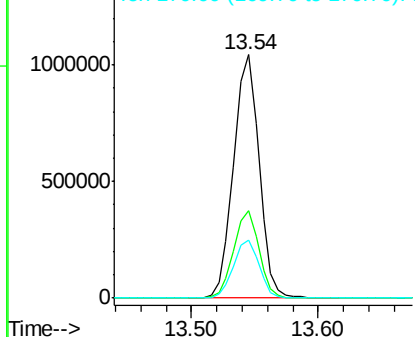


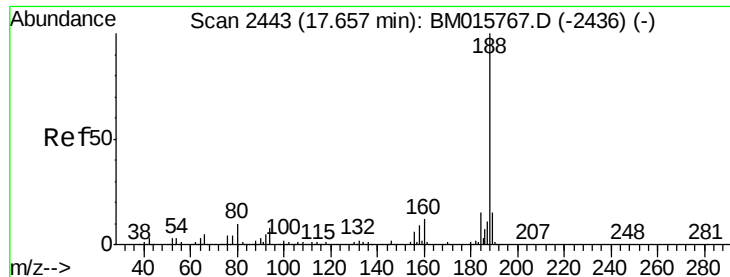

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.64 min Scan# 2441
Delta R.T. -0.01 min
Lab File: BM015882.D
Acq: 10 Jul 2018 23:53




Instrument :
BNA_M
ClientSampleId :
PB110959BL


Tgt Ion:188 Resp: 414841
Ion Ratio Lower Upper
188 100
94 7.8 8.7 13.1#
80 9.2 9.3 13.9#

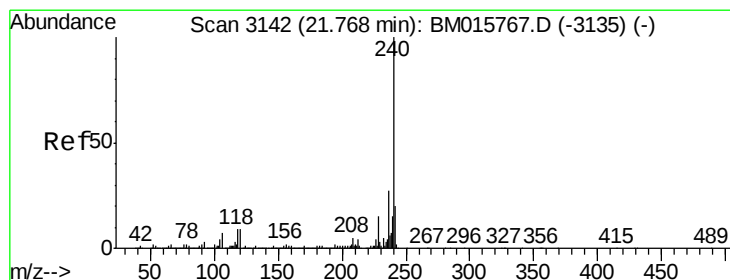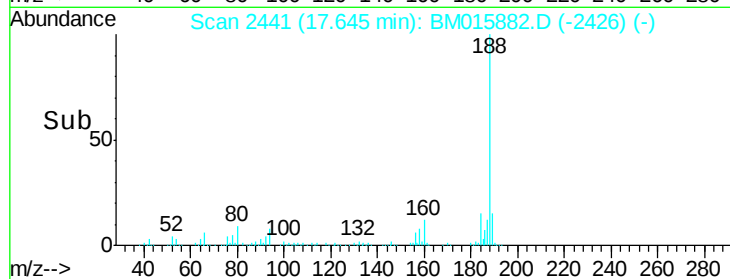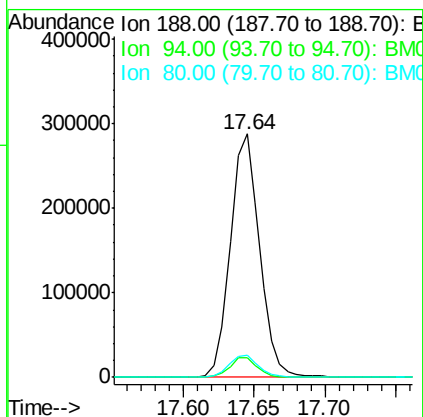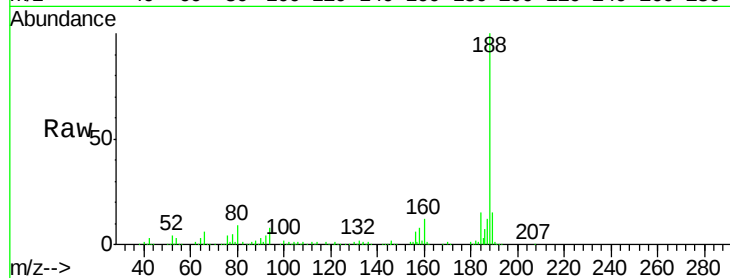

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.75 min Scan# 3139
Delta R.T. -0.02 min
Lab File: BM015882.D
Acq: 10 Jul 2018 23:53

Tgt Ion:240 Resp: 405574
Ion Ratio Lower Upper
240 100
120 9.3 8.2 12.2
236 27.4 20.0 30.0

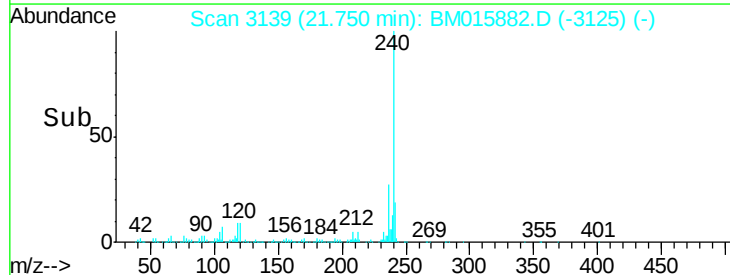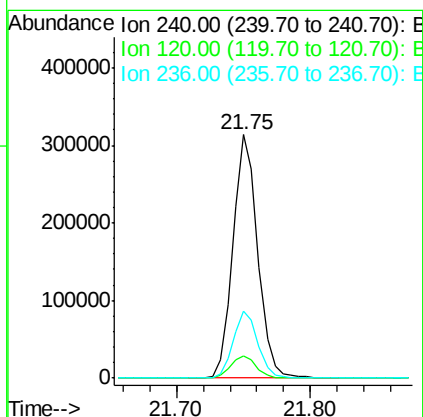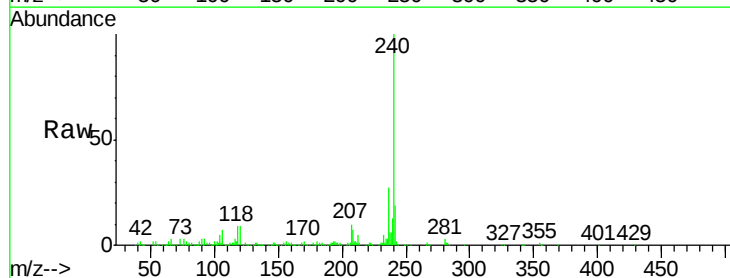

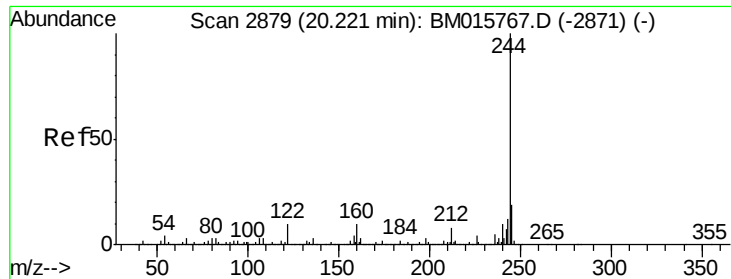

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.21 min Scan# 2877

Delta R.T. -0.01 min

Lab File: BM015882.D

Acq: 10 Jul 2018 23:53

Instrument :

BNA_M

ClientSampleId :

PB110959BL


Tgt Ion:244 Resp: 2795322

Ion Ratio Lower Upper

244 100

212 8.4 4.9 7.3#




122 9.4 6.2 9.4#

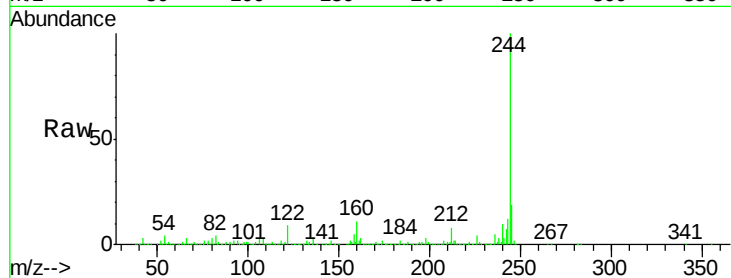

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

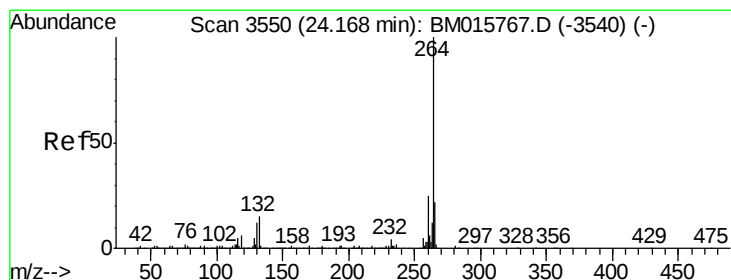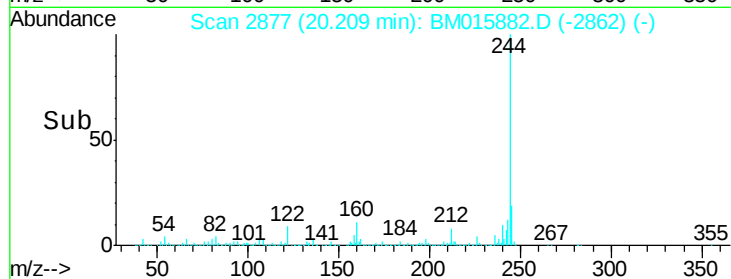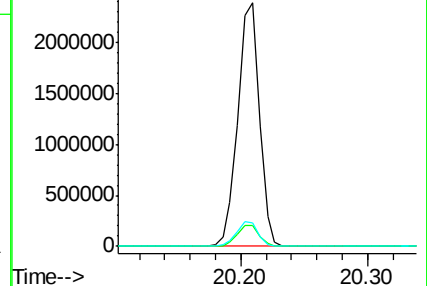

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.15 min Scan# 3547

Delta R.T. -0.02 min

Lab File: BM015882.D

Acq: 10 Jul 2018 23:53


Tgt Ion:264 Resp: 372028

Ion Ratio Lower Upper

264 100

260 24.7 18.6 27.8

265 21.0 17.3 25.9

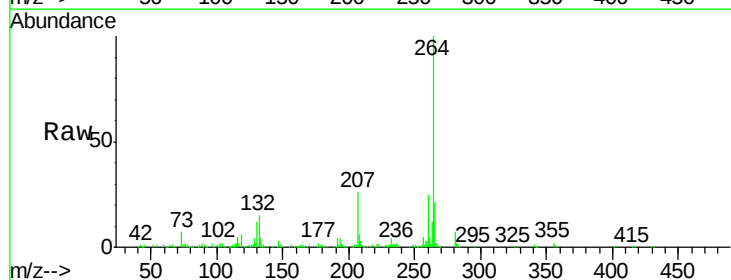

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

