
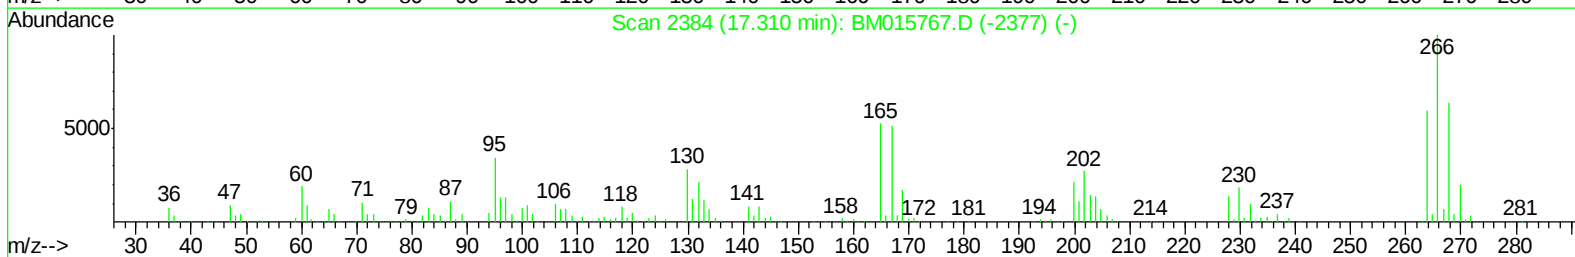
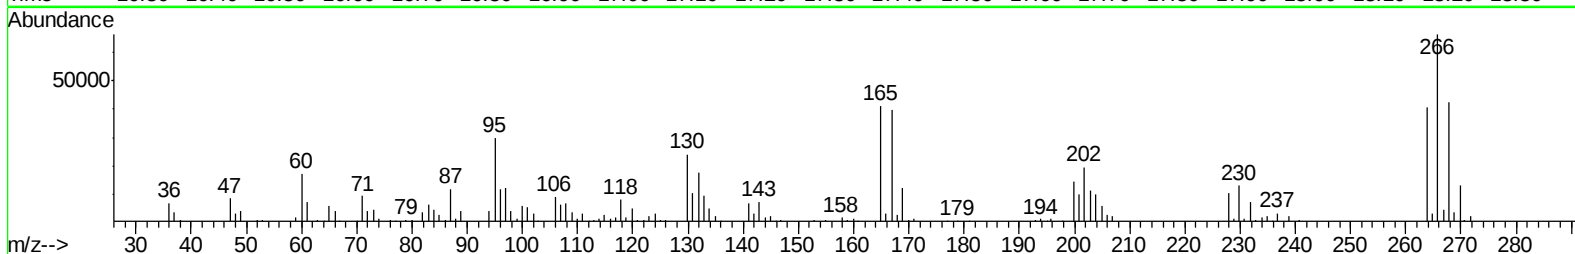


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM071018\  
Data File : BM015869.D  
Acq On : 10 Jul 2018 15:49  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 04:56:05 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM070518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 05 17:39:50 2018  
Response via : Initial Calibration

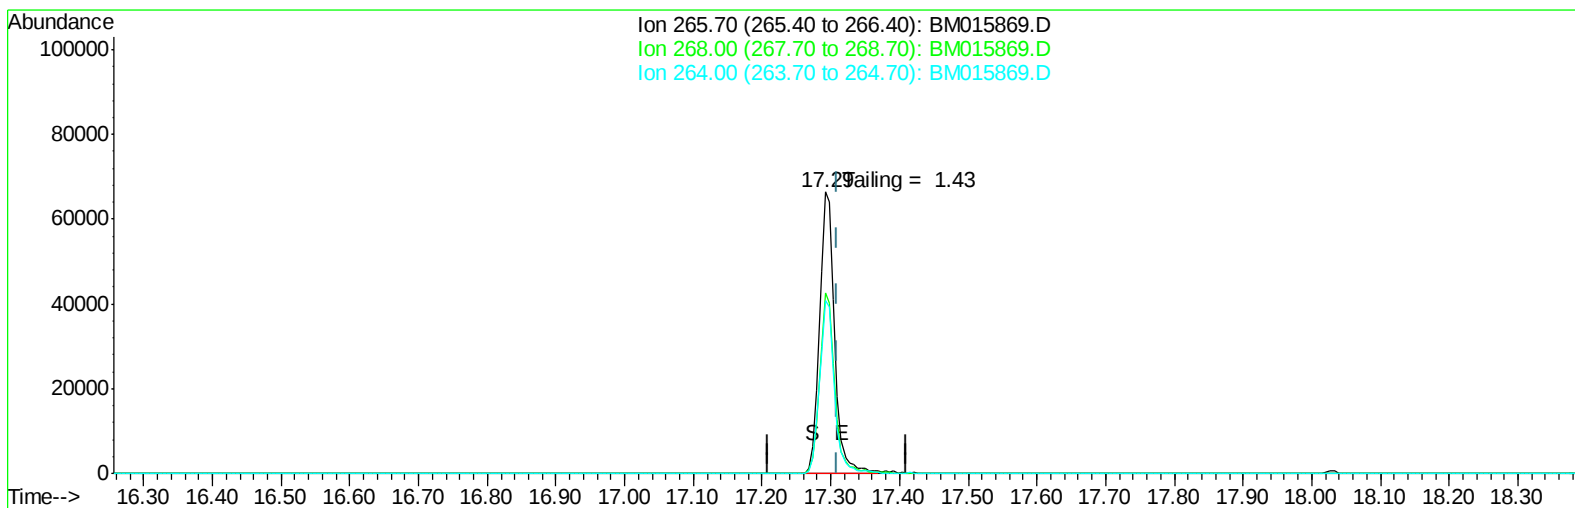

TIC: BM015869.D

(69) Pentachlorophenol (C)




17.292min (-0.018) 0.00ng

response 101658

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 63.95 |
| 264.00 | 61.20 | 61.20 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM071018\  
Data File : BM015869.D  
Acq On : 10 Jul 2018 15:49  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 04:56:05 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM070518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 05 17:39:50 2018  
Response via : Initial Calibration

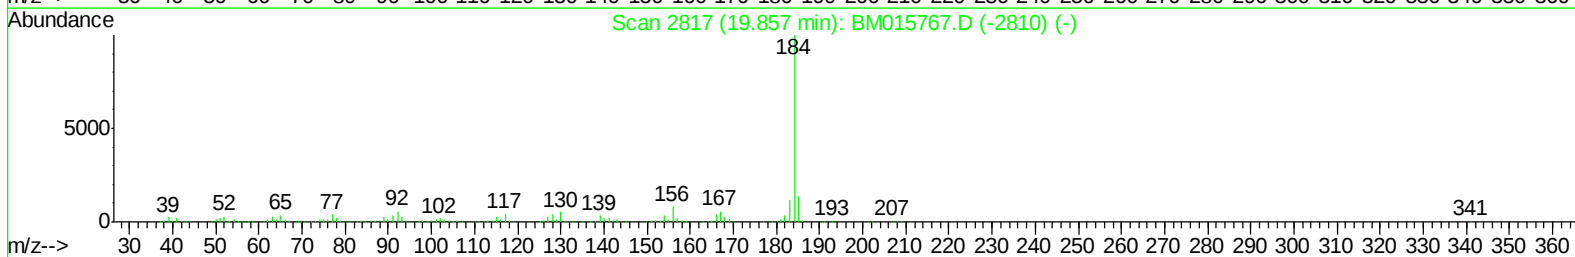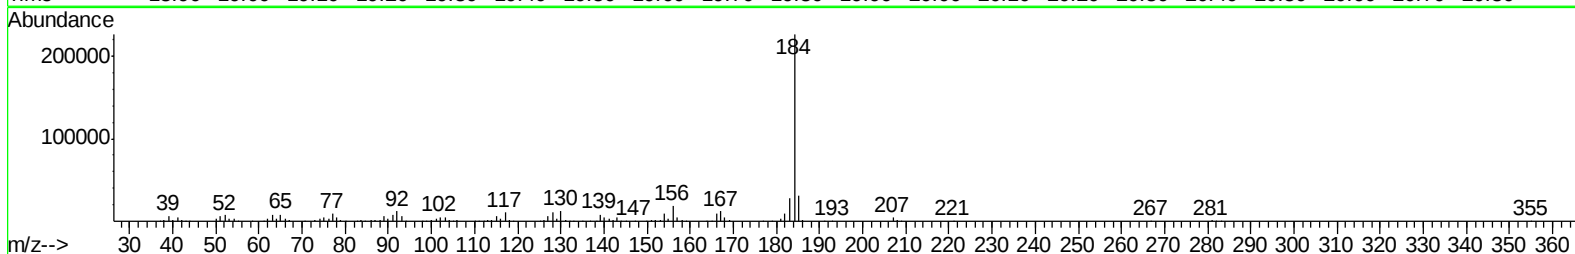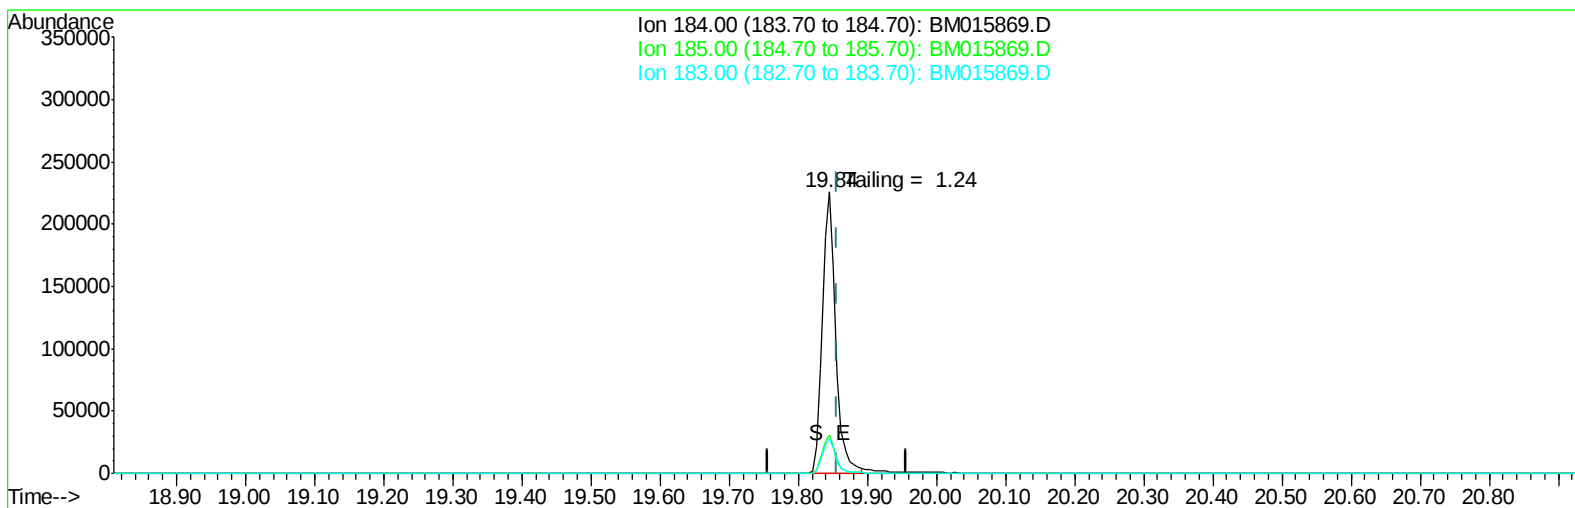

TIC: BM015869.D

(76) Benzidine

19.845min (-0.012) 2536.23ng

response 303998

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 13.77 |
| 183.00 | 11.10 | 12.46 |
| 0.00   | 0.00  | 0.00  |