

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071018\
 Data File : BM015877.D
 Acq On : 10 Jul 2018 20:47
 Operator : SJ/JU
 Sample : J3914-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B3

Quant Time: Jul 11 03:47:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 05 17:39:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	63420	20.00	ng	-0.02
21) Naphthalene-d8	11.12	136	259189	20.00	ng	-0.02
38) Acenaphthene-d10	14.92	164	156394	20.00	ng	-0.02
63) Phenanthrene-d10	17.64	188	385813	20.00	ng	-0.01
75) Chrysene-d12	21.75	240	385888	20.00	ng	-0.02
86) Perylene-d12	24.14	264	243378	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	566286	153.13	ng	-0.02
7) Phenol-d6	7.45	99	692342	136.76	ng	-0.02
23) Nitrobenzene-d5	9.48	82	534613	100.64	ng	-0.02
41) 2,4,6-Tribromophenol	16.40	330	362310	177.30	ng	-0.02
44) 2-Fluorobiphenyl	13.54	172	1194513	94.82	ng	-0.02
78) Terphenyl-d14	20.20	244	2575691	123.81	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071018\
Data File : BM015877.D
Acq On : 10 Jul 2018 20:47
Operator : SJ/JU
Sample : J3914-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B3

Quant Time: Jul 11 03:47:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

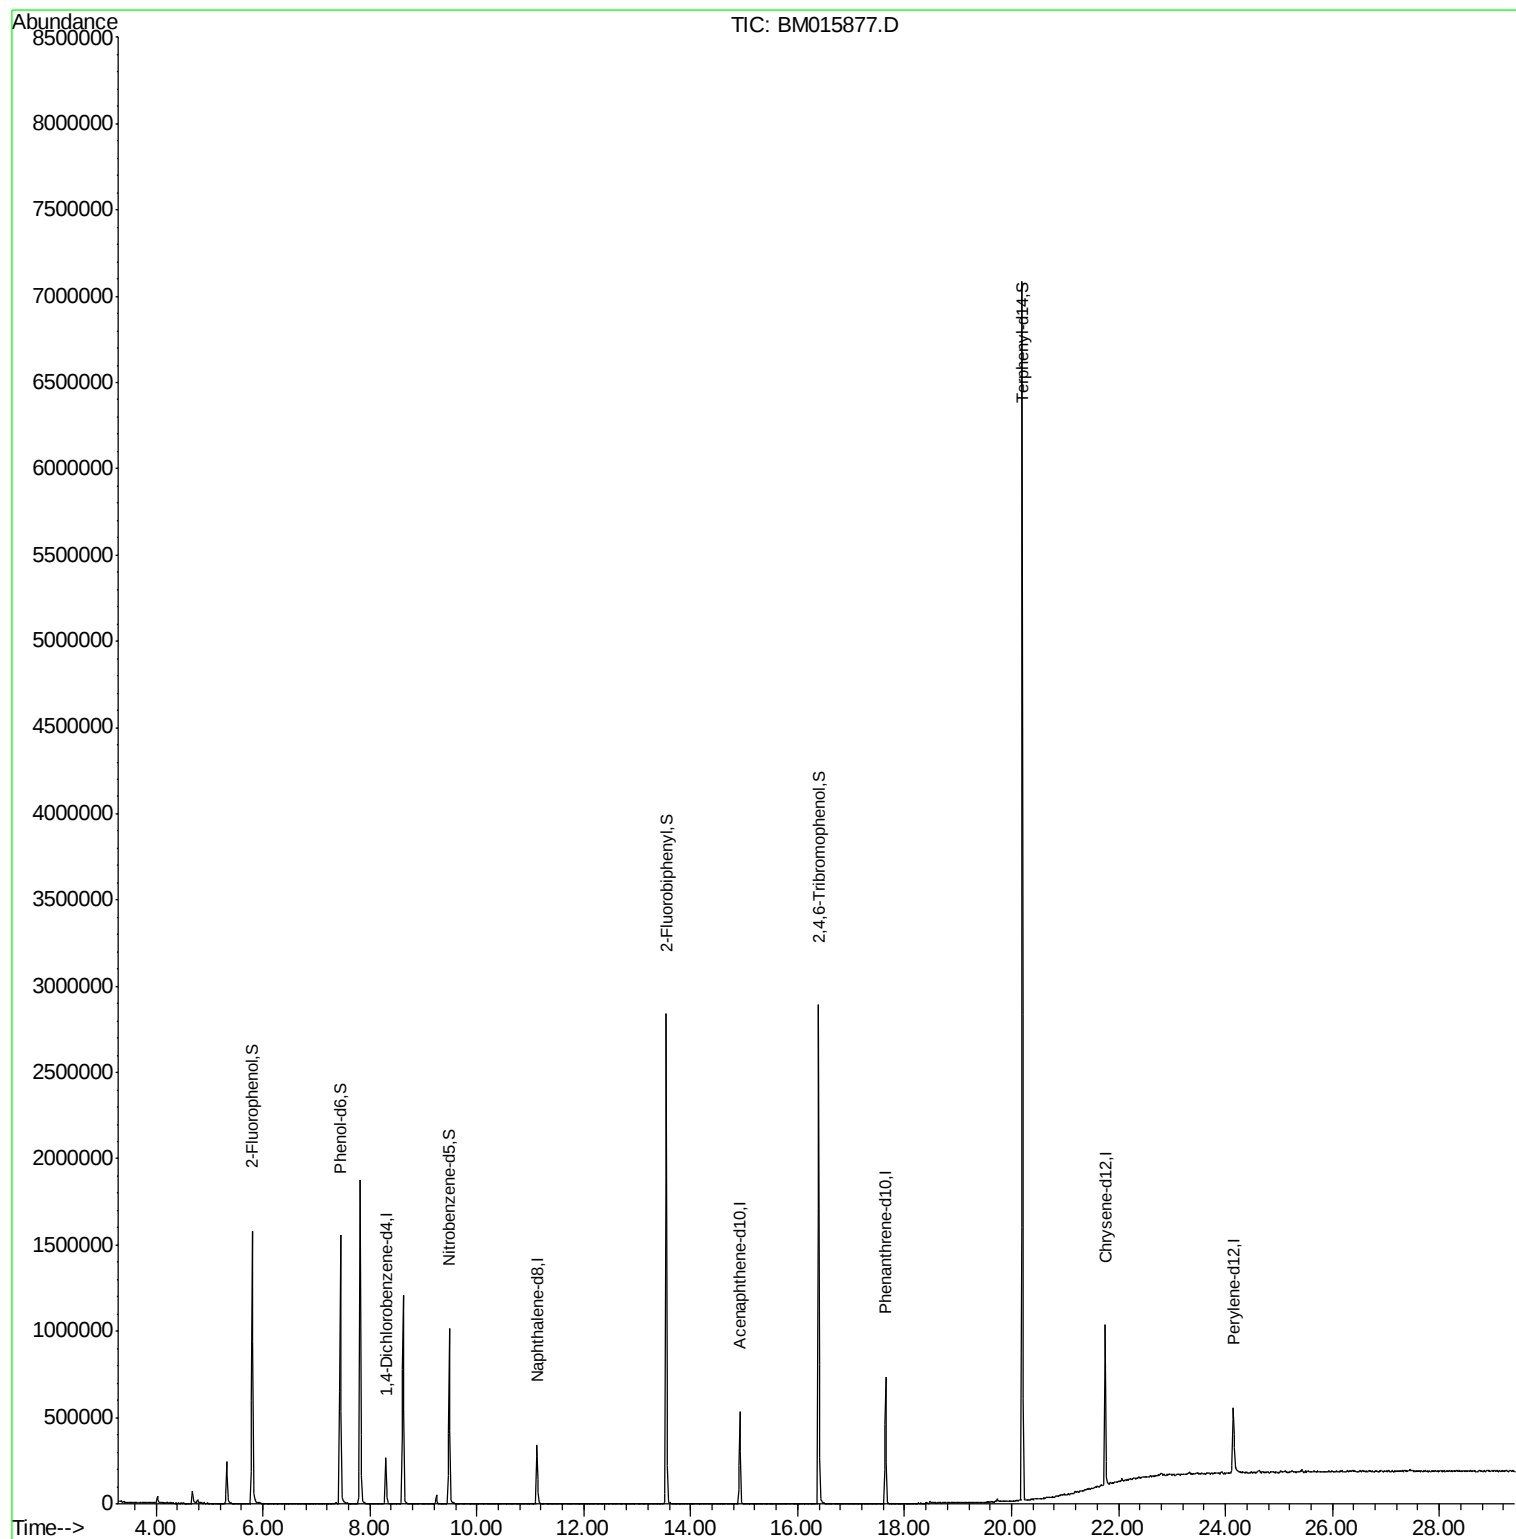

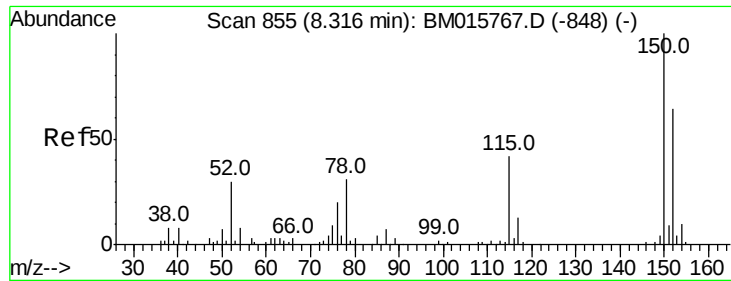


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.30 min Scan# 852
Delta R.T. -0.02 min
Lab File: BM015877.D
Acq: 10 Jul 2018 20:47

Instrument :
BNA_M
ClientSampled :
B3

Tot Ion:152 Resp: 63420
Ion Ratio Lower Upper
152 100
150 151.4 119.5 179.3
115 65.7 43.0 64.4#

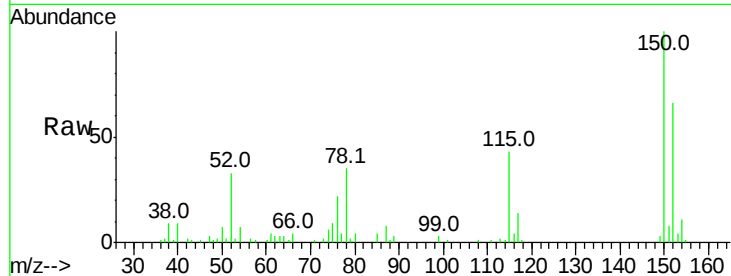


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

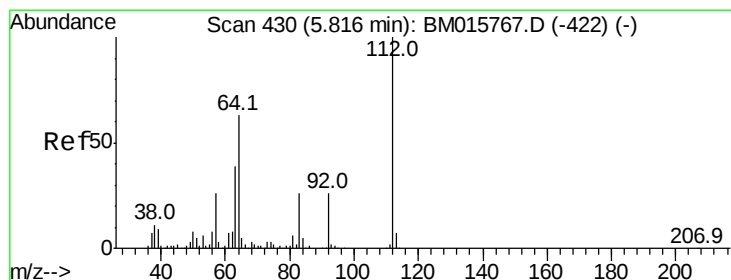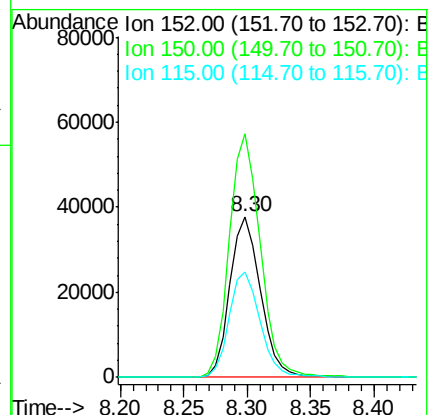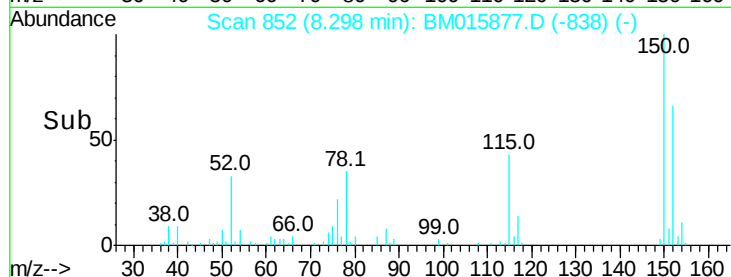



#5


2-Fluorophenol
Concen: Below ng
RT: 5.80 min Scan# 427
Delta R.T. -0.02 min
Lab File: BM015877.D
Acq: 10 Jul 2018 20:47

Tgt Ion:112 Resp: 566286
Ion Ratio Lower Upper
112 100
64 63.9 38.6 57.8#
63 42.1 19.3 28.9#

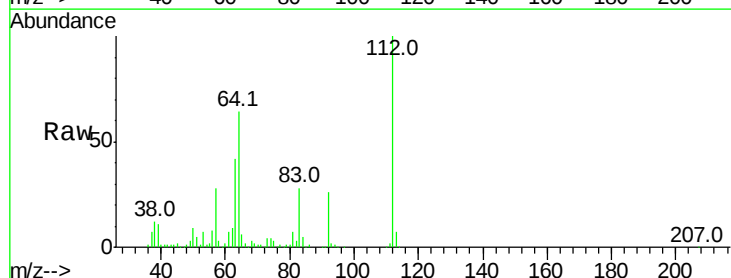

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

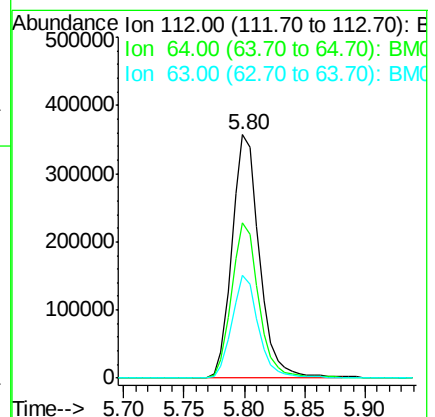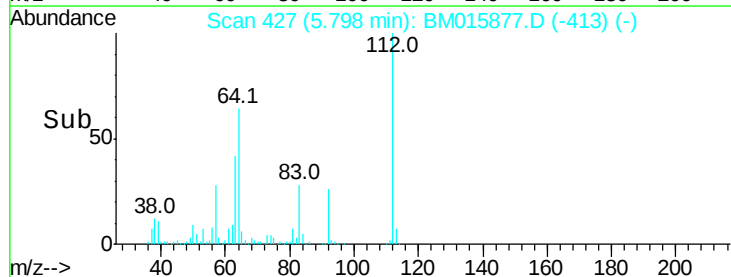

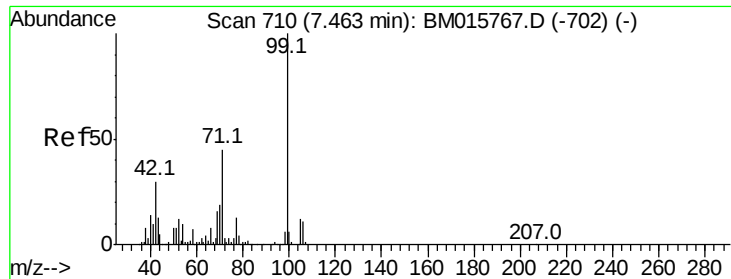

#7

Phenol-d6

Concen: N.D. ng

RT: 7.45 min Scan# 707

Delta R.T. -0.02 min

Lab File: BM015877.D

Acq: 10 Jul 2018 20:47

Instrument :

BNA_M

ClientSampleId :

B3


Tot Ion: 99 Resp: 692342

Ion Ratio Lower Upper

99 100

42 32.8 11.0 16.4#

71 47.9 23.4 35.2#

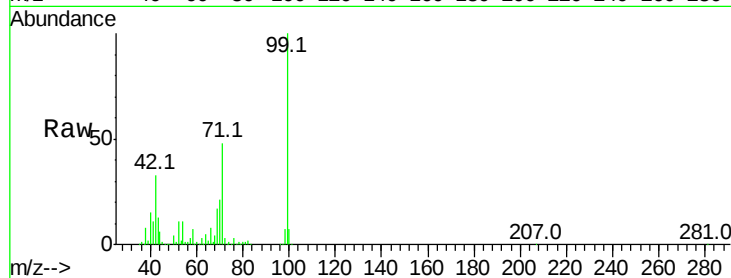

Abundance Ion 99.00 (98.70 to 99.70): BM015877.D (-693) (-)

Ion 42.00 (41.70 to 42.70): BM015877.D (-693) (-)

Ion 71.00 (70.70 to 71.70): BM015877.D (-693) (-)

7.45

400000



300000

200000

100000

0

Time--> 7.35 7.40 7.45 7.50 7.55

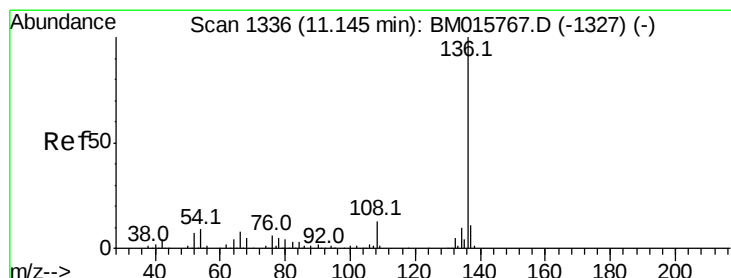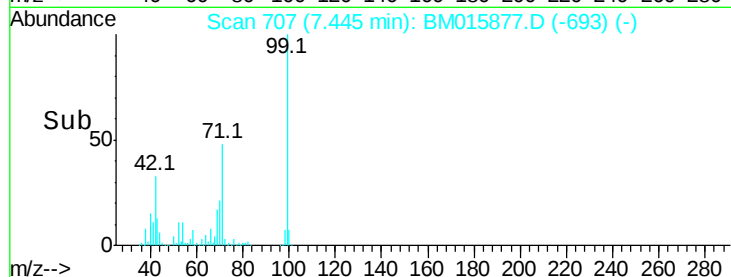

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.12 min Scan# 1332

Delta R.T. -0.02 min

Lab File: BM015877.D

Acq: 10 Jul 2018 20:47

Tgt Ion: 136 Resp: 259189


Ion Ratio Lower Upper

136 100

137 10.7 8.7 13.1

54 10.0 4.6 6.8#

68 4.5 3.7 5.5

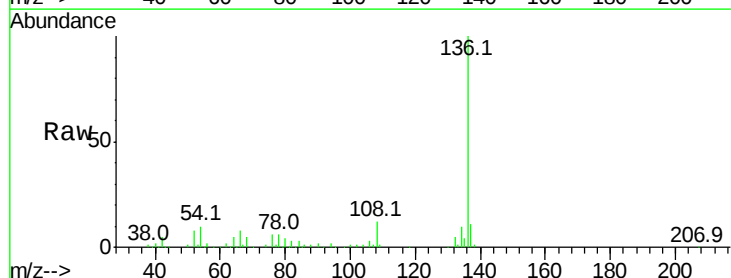

Abundance Ion 136.00 (135.70 to 136.70): BM015877.D (-1319) (-)

Ion 137.00 (136.70 to 137.70): BM015877.D (-1319) (-)

Ion 54.00 (53.70 to 54.70): BM015877.D (-1319) (-)

Ion 68.00 (67.70 to 68.70): BM015877.D (-1319) (-)

11.12

200000


150000


100000

50000

0

Time--> 11.10 11.20




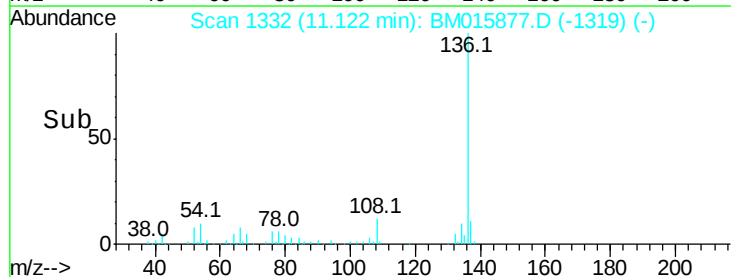


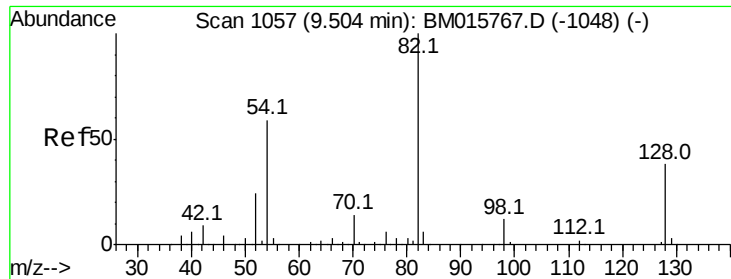

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.48 min Scan# 1053
Delta R.T. -0.02 min
Lab File: BM015877.D
Acq: 10 Jul 2018 20:47




Instrument :
BNA_M
ClientSampled :
B3


Tot Ion: 82 Resp: 534613
Ion Ratio Lower Upper
82 100
128 36.6 32.8 49.2
54 61.4 40.6 60.8#

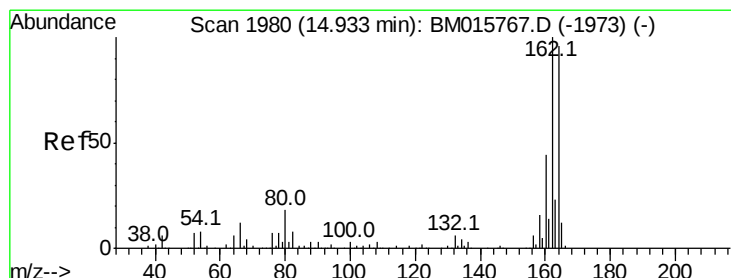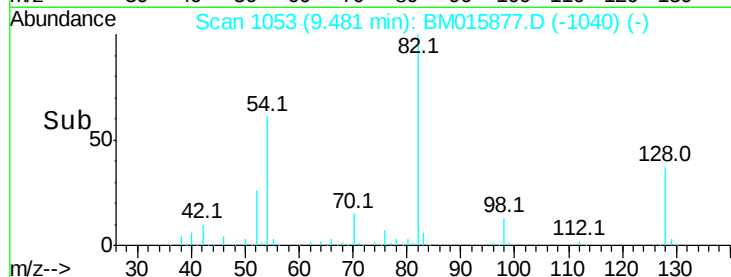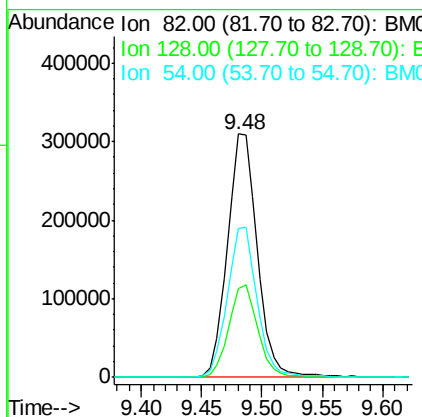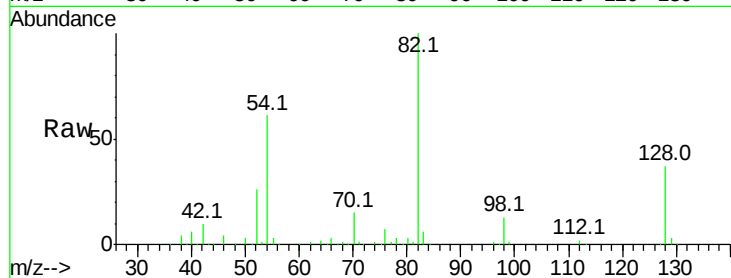

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.92 min Scan# 1977
Delta R.T. -0.02 min
Lab File: BM015877.D
Acq: 10 Jul 2018 20:47

Tgt Ion: 164 Resp: 156394
Ion Ratio Lower Upper
164 100
162 105.7 82.4 123.6
160 47.8 35.8 53.6

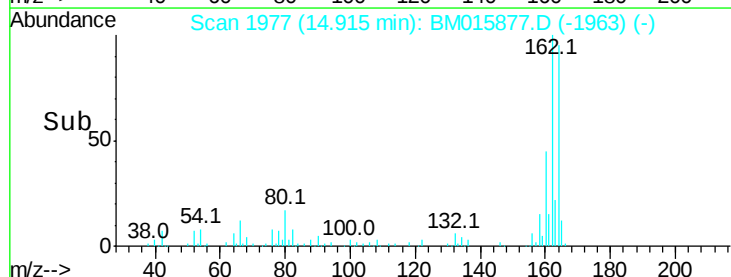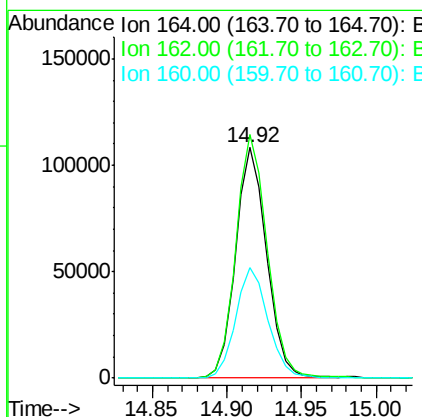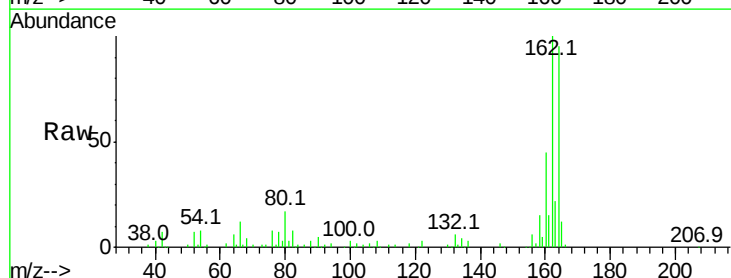


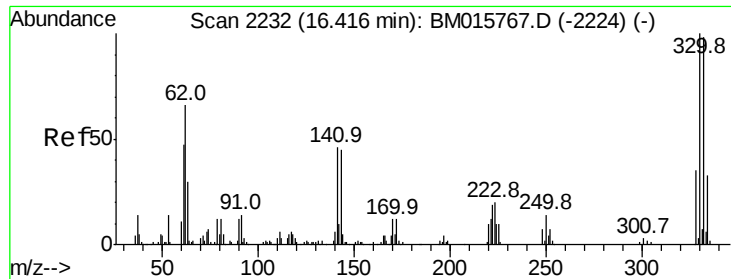




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.40 min Scan# 2229
 Delta R.T. -0.02 min
 Lab File: BM015877.D
 Acq: 10 Jul 2018 20:47

Instrument :
 BNA_M
 ClientSampleId :
 B3

Tot Ion:330 Resp: 362310
 Ion Ratio Lower Upper
 330 100
 332 96.7 0.0 0.0#
 141 57.9 0.0 0.0#

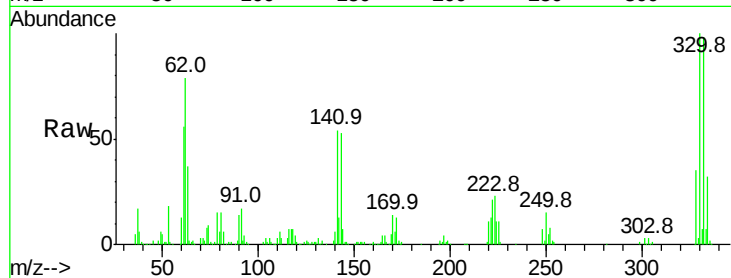


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

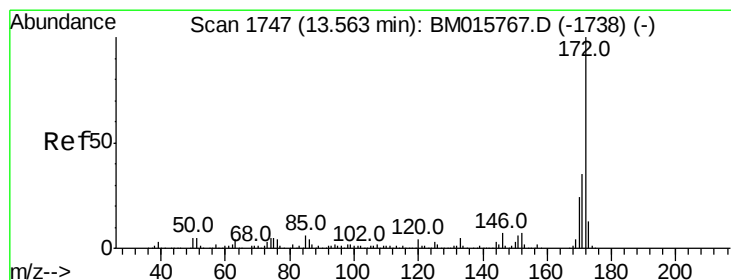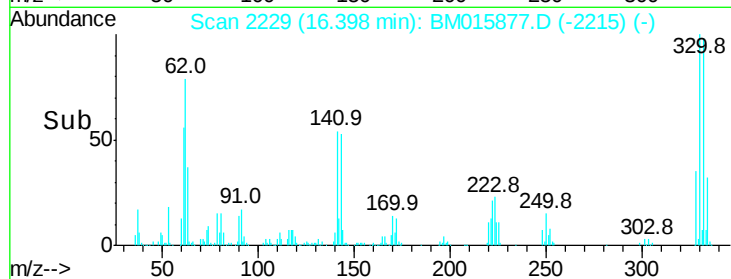
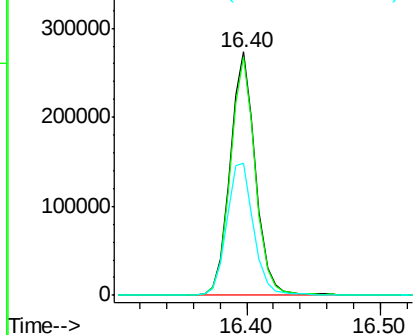



#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.54 min Scan# 1744
 Delta R.T. -0.02 min
 Lab File: BM015877.D
 Acq: 10 Jul 2018 20:47

Tgt Ion:172 Resp: 1194513
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.5 42.7
 170 23.9 18.8 28.2

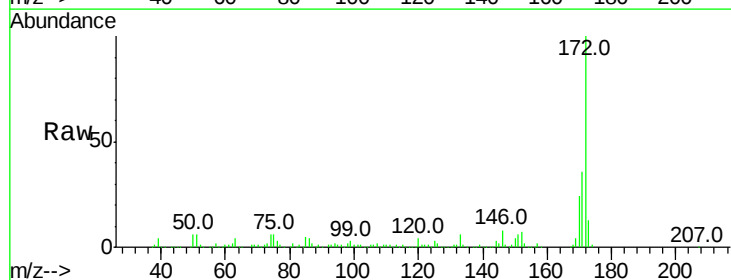

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



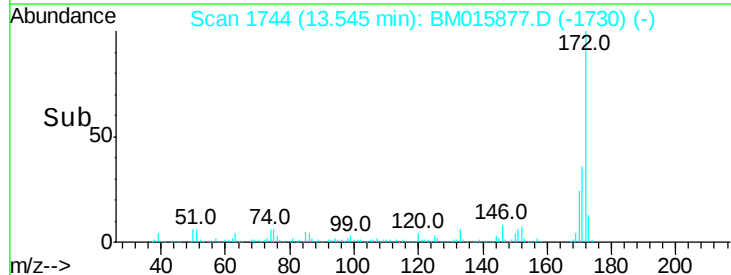
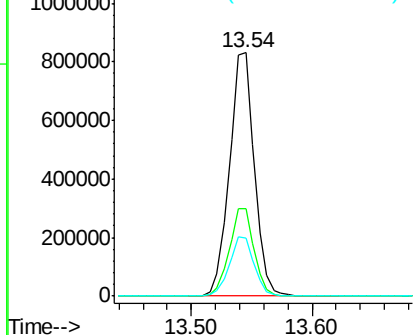


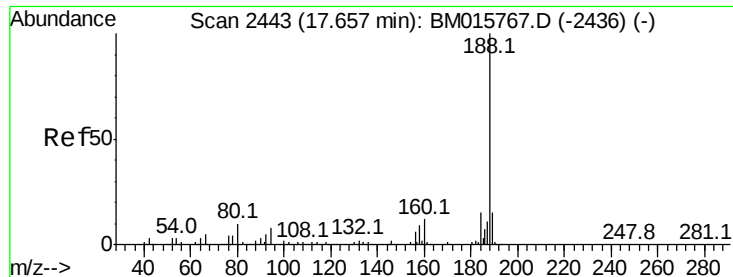

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.64 min Scan# 2441
Delta R.T. -0.01 min
Lab File: BM015877.D
Acq: 10 Jul 2018 20:47




Instrument :
BNA_M
ClientSampleId :
B3


Tot Ion:188 Resp: 385813
Ion Ratio Lower Upper
188 100
94 7.3 8.7 13.1#
80 8.3 9.3 13.9#

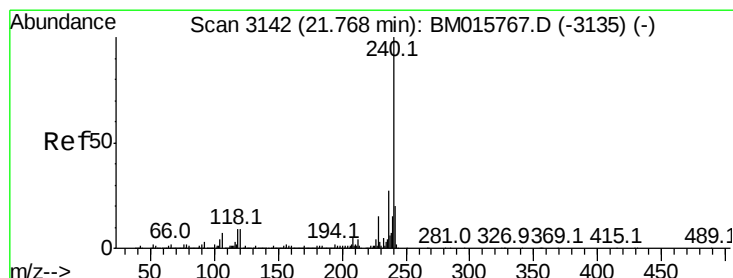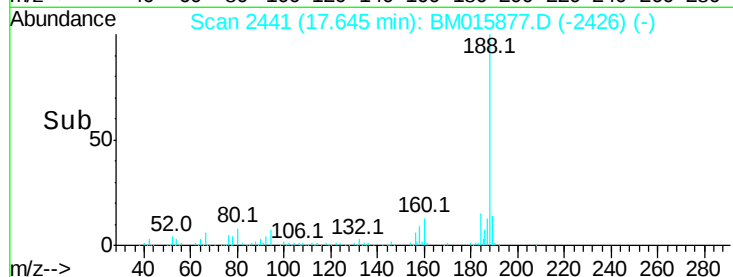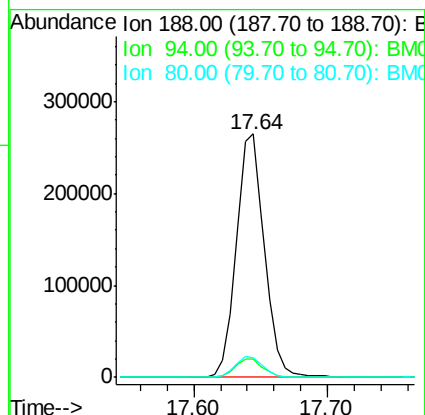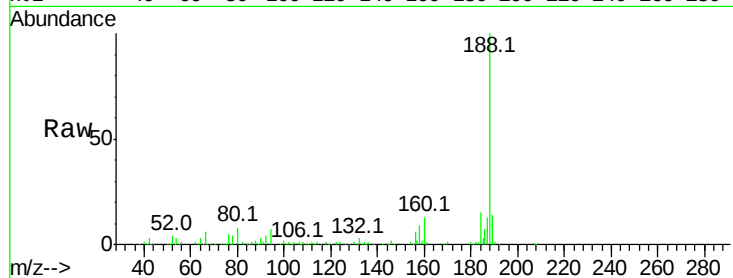

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.75 min Scan# 3139
Delta R.T. -0.02 min
Lab File: BM015877.D
Acq: 10 Jul 2018 20:47

Tgt Ion:240 Resp: 385888
Ion Ratio Lower Upper
240 100
120 9.4 8.2 12.2
236 27.4 20.0 30.0


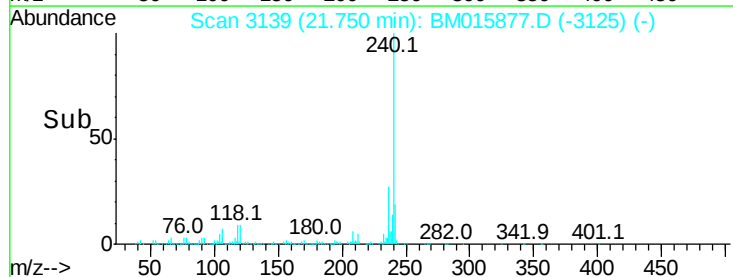
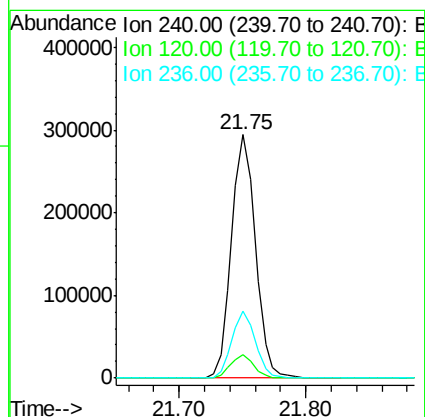
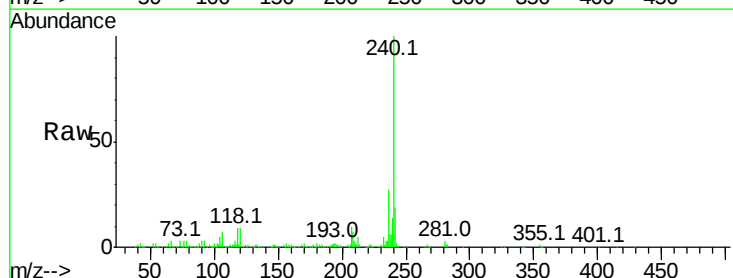


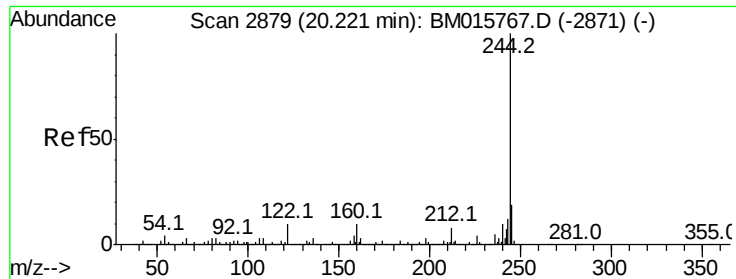

#78
 Terphenyl-d14
 Concen: N.D. ng
 RT: 20.20 min Scan# 2876
 Delta R.T. -0.02 min
 Lab File: BM015877.D
 Acq: 10 Jul 2018 20:47

Instrument :
 BNA_M
 ClientSampled :
 B3

Tot Ion:244 Resp: 2575691
 Ion Ratio Lower Upper
 244 100
 212 8.7 4.9 7.3#
 122 10.3 6.2 9.4#

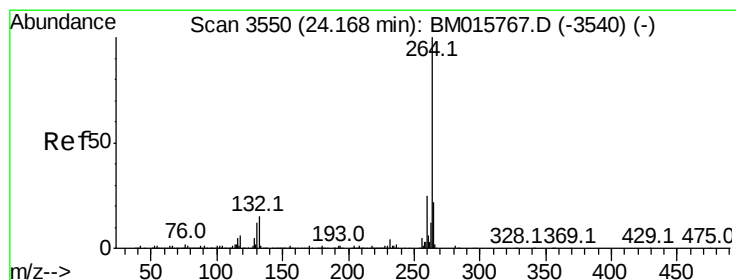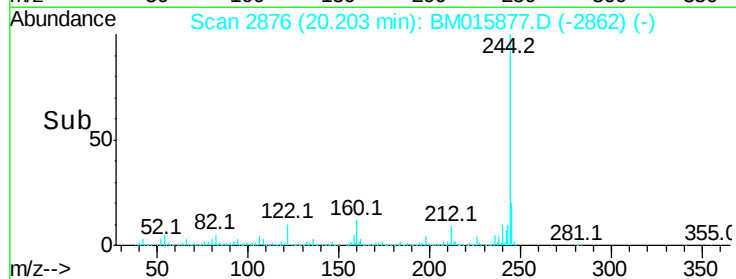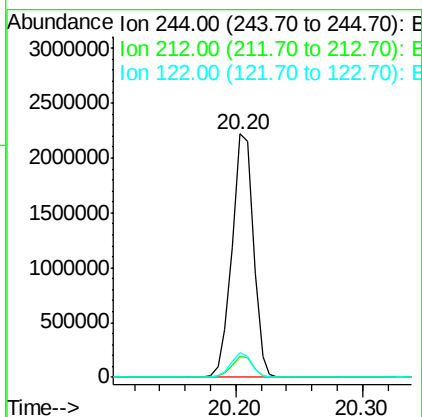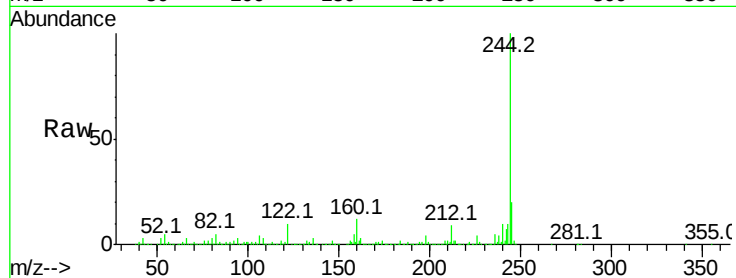

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.14 min Scan# 3546
 Delta R.T. -0.02 min
 Lab File: BM015877.D
 Acq: 10 Jul 2018 20:47

Tgt Ion:264 Resp: 243378
 Ion Ratio Lower Upper
 264 100
 260 26.0 18.6 27.8
 265 21.6 17.3 25.9

