


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071018\
 Data File : BM015869.D
 Acq On : 10 Jul 2018 15:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

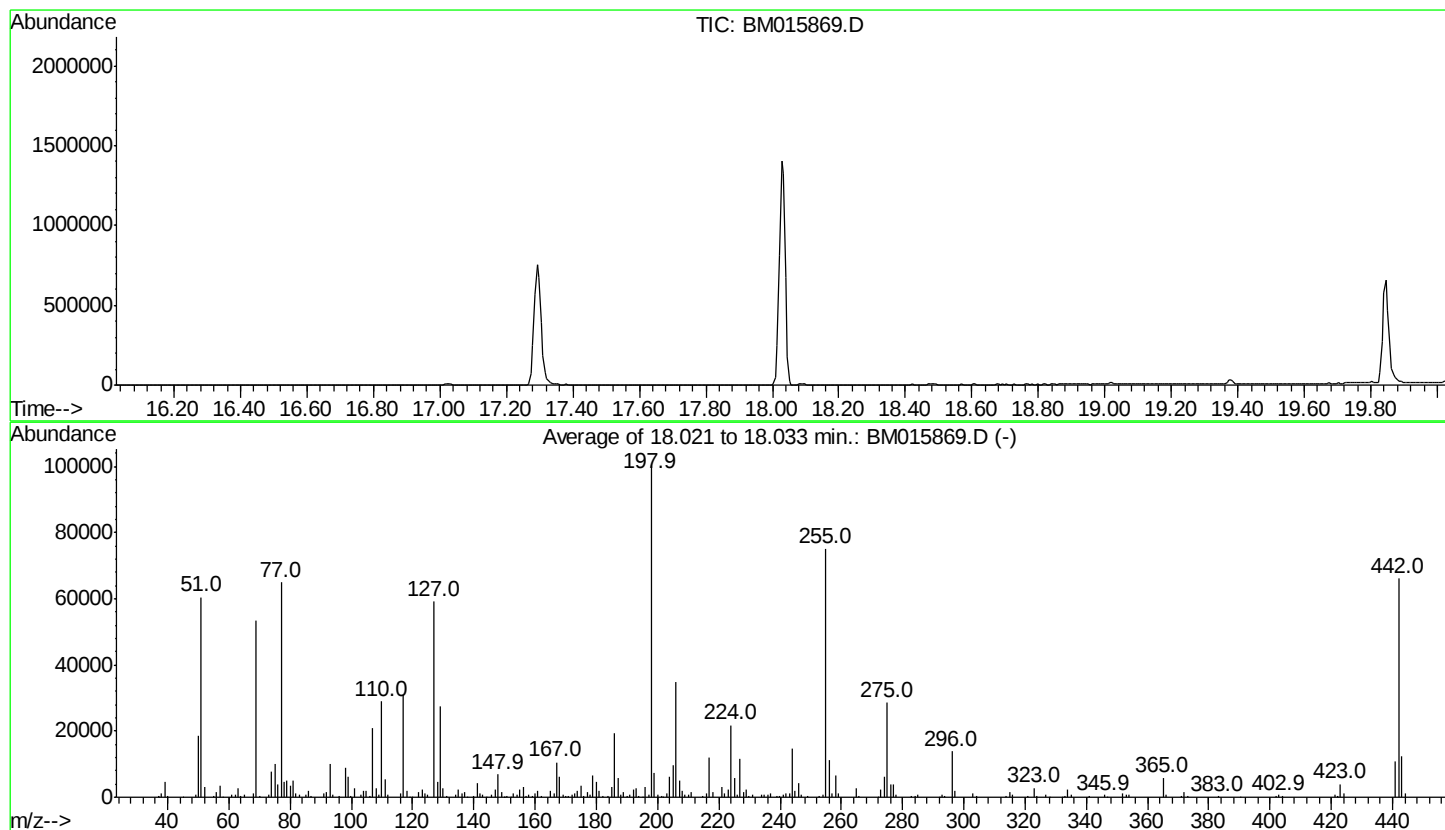

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.2	60373	PASS
68	69	0.00	2	2.0	1068	PASS
69	198	0.00	100	53.3	53426	PASS
70	69	0.00	2	0.4	216	PASS
127	198	10	80	58.9	59064	PASS
197	198	0.00	2	0.7	718	PASS
198	198	100	100	100.0	100224	PASS
199	198	5	9	7.2	7249	PASS
275	198	10	60	28.4	28510	PASS
365	198	1	100	6.0	6010	PASS
441	443	0.01	100	85.0	10681	PASS
442	198	50	100	65.8	65994	PASS
443	442	15	24	19.1	12572	PASS