

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
 Data File : BM021418.D
 Acq On : 10 Jul 2019 21:43
 Operator : HP/JU
 Sample : K3717-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF4C7

Manual Integrations
 APPROVED

mohammad
 7/11/2019 5:23:22 PM

Quant Time: Jul 11 01:48:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 08 17:45:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	180771	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	712186	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.38	164	419041	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	973923	20.00	ng/ul	0.00
77) Chrysene-d12	21.31	240	917896	20.00	ng/ul	0.00
85) Perylene-d12	23.57	264	1023885	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	22202	6.05	ng/uL	0.00
5) Phenol-d5	6.91	99	78432	5.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	195643	23.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	241267	19.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	145445	12.99	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	143963	24.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	157166	23.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	289529	21.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	23794m	1.99	ng/ul	0.01
43) Dimethylphthalate-d6	13.79	166	1030448	28.08	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	1154805	25.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	22741m	3.91	ng/ul	0.00
57) Fluorene-d10	15.37	176	962331	29.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	139698	21.34	ng/ul	0.00
70) Anthracene-d10	17.23	188	1629614	32.21	ng/ul	0.00
78) Pyrene-d10	19.53	212	1837630	36.48	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.43	264	1969367	33.44	ng/ul	0.00

Target Compounds

					Ovalue
4) Benzaldehyde	6.90	77	13766	1.814	ng/ul 91
33) 4-Chloro-3-methylphenol	11.83	107	19163	1.701	ng/ul 93
44) Dimethylphthalate	13.84	163	70539	2.064	ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
Data File : BM021418.D
Acq On : 10 Jul 2019 21:43
Operator : HP/JU
Sample : K3717-06
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF4C7

Quant Time: Jul 11 01:48:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 08 17:45:45 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
7/11/2019 5:23:22 PM

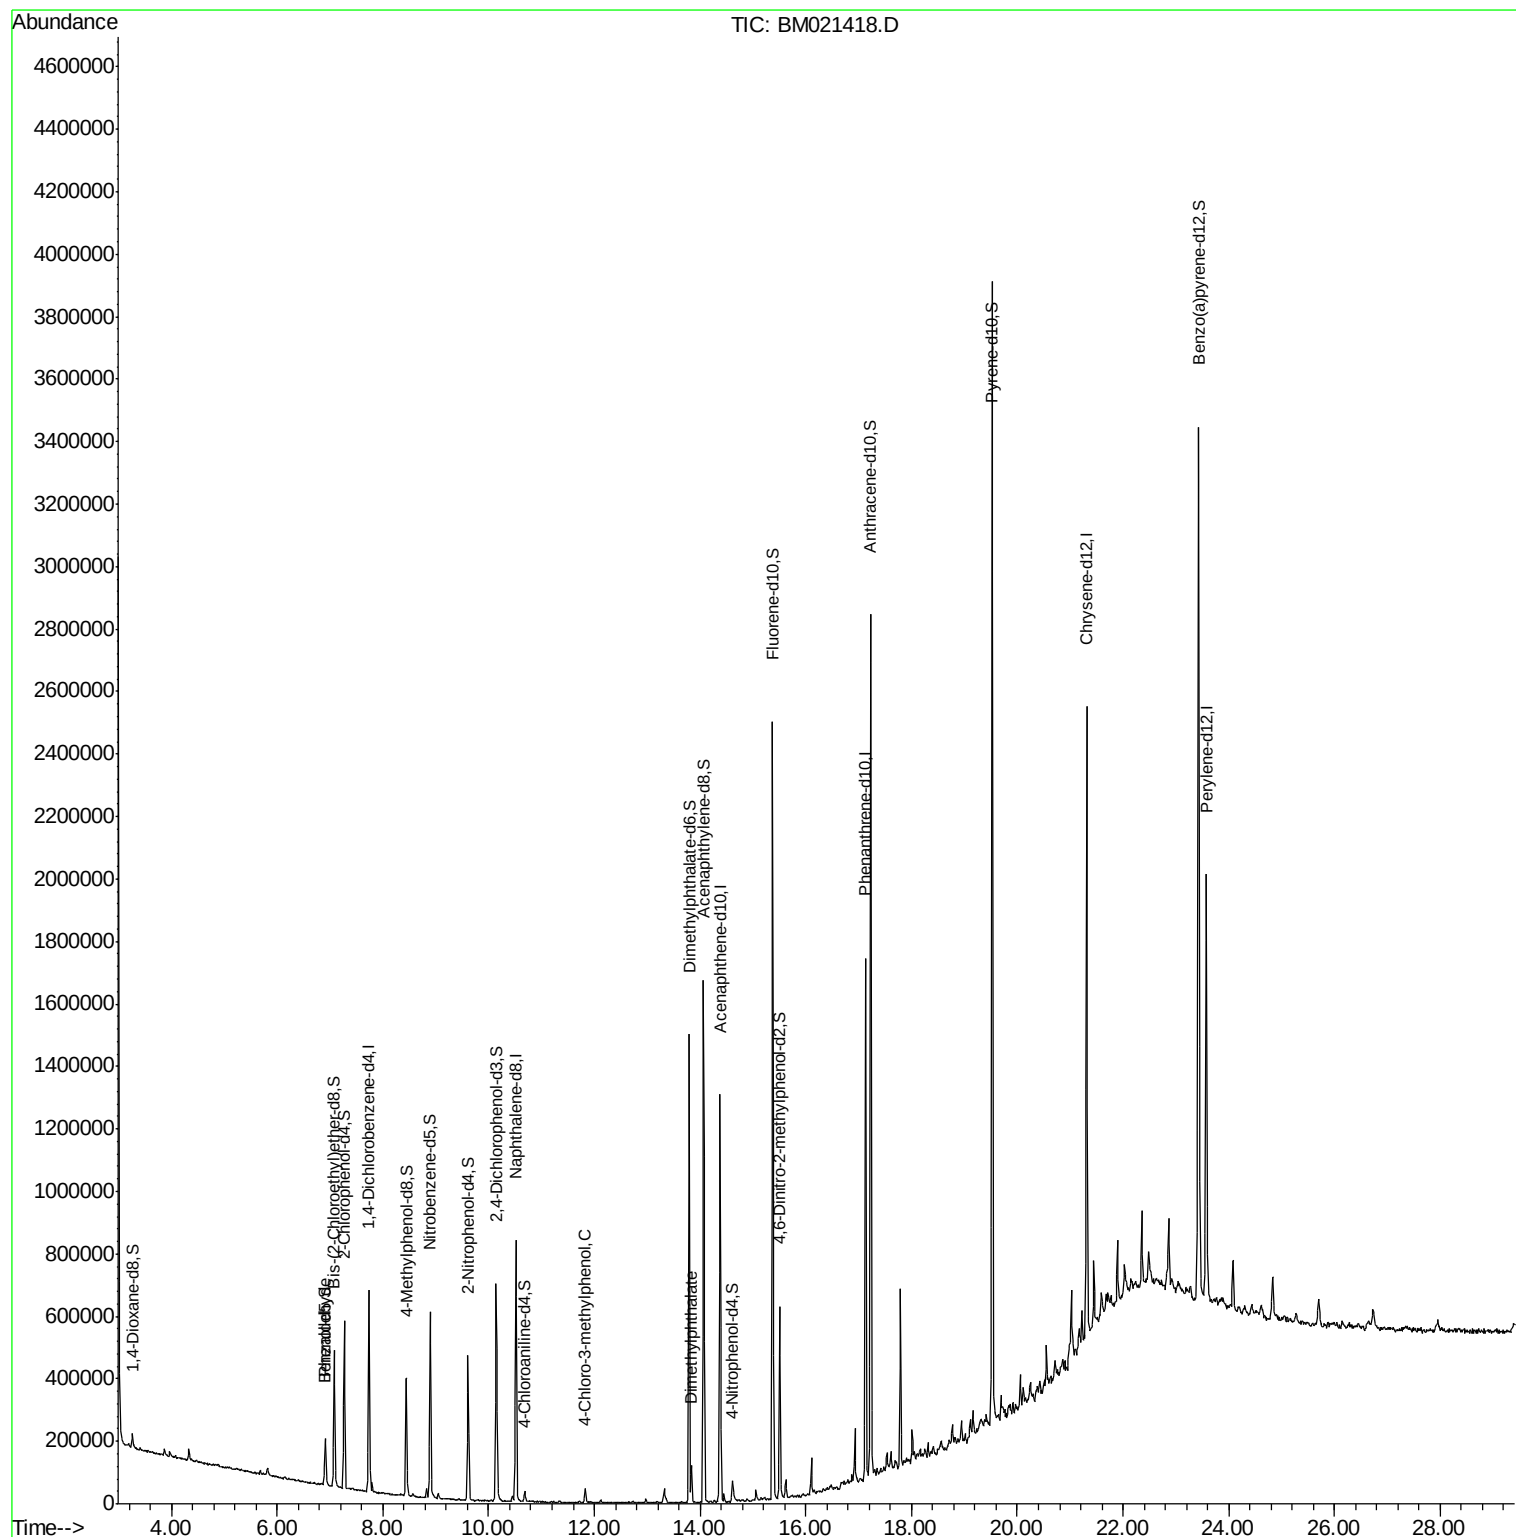

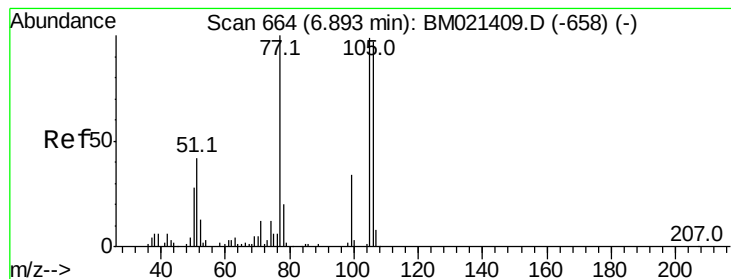

#4

Benzaldehyde

Concen: 1.814 ng/ul

RT: 6.90 min Scan# 665

Delta R.T. 0.01 min

Lab File: BM021418.D

Acq: 10 Jul 2019 21:43

Instrument :

BNA_M





ClientSampled :

BF4C7

Tot Ion:	77	Resp:	13766
Ion	Ratio	Lower	Upper
77	100		
105	84.2	76.8	115.2
106	84.2	71.4	107.2

Manual Integrations
APPROVED

mohammad
7/11/2019 5:23:22 PM

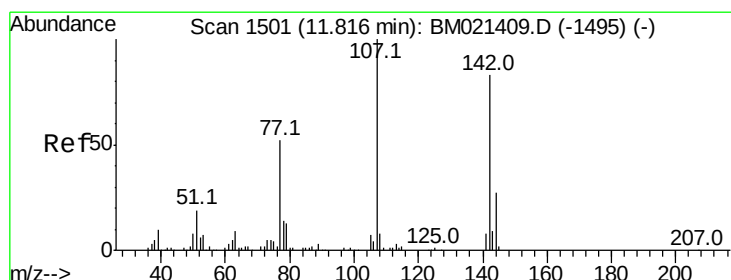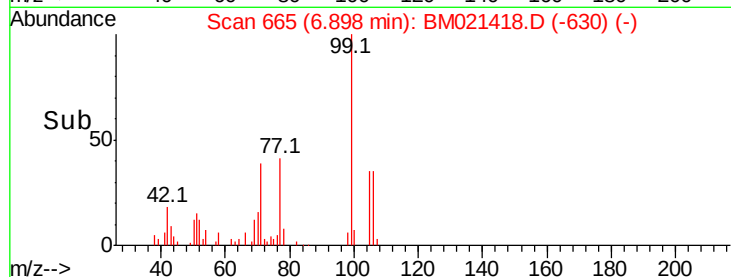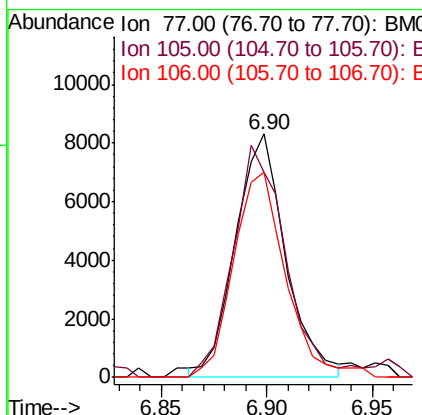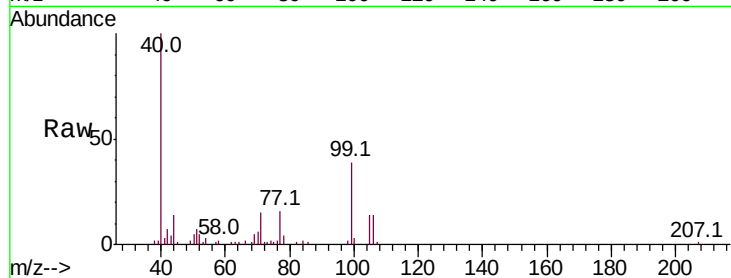

#33

4-Chloro-3-methylphenol

Concen: 1.701 ng/ul




RT: 11.83 min Scan# 1503


Delta R.T. 0.01 min

Lab File: BM021418.D

Acq: 10 Jul 2019 21:43

Tgt Ion:	107	Resp:	19163
Ion	Ratio	Lower	Upper
107	100		
144	26.6	21.4	32.2
142	89.1	64.7	97.1

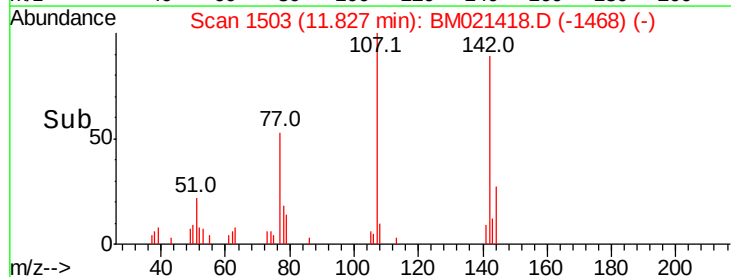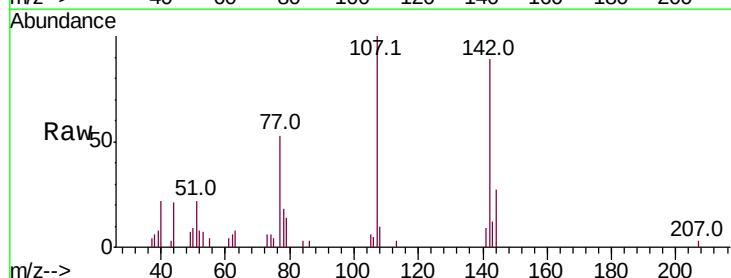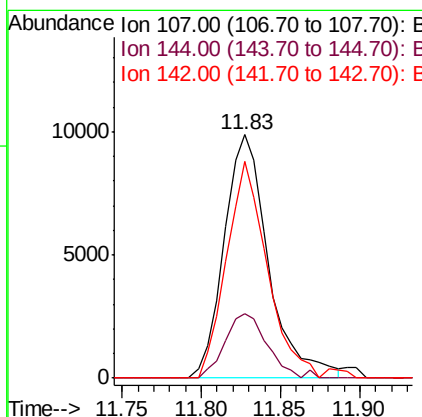

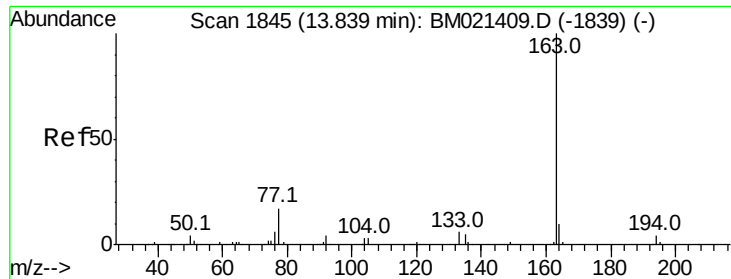

#44
 Dimethylphthalate
 Concen: 2.064 ng/ul
 RT: 13.84 min Scan# 1845
 Delta R.T. -0.00 min
 Lab File: BM021418.D
 Acq: 10 Jul 2019 21:43

Instrument :
 BNA_M
 ClientSampleId :
 BF4C7

Tot Ion:163	Resp:	70539
Ion Ratio	Lower	Upper
163 100		
194 4.4	3.6	5.4
164 9.0	8.3	12.5

Manual Integrations
 APPROVED

mohammad
 7/11/2019 5:23:22 PM

