

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
 Data File : BM021423.D
 Acq On : 11 Jul 2019 02:00
 Operator : HP/JU
 Sample : K3717-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF4A3

Manual Integrations
 APPROVED

mohammad
 7/11/2019 5:23:35 PM

Quant Time: Jul 11 04:52:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 08 17:45:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	162679	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	621037	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	365172	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	862563	20.00	ng/ul	0.00
77) Chrysene-d12	21.32	240	855125	20.00	ng/ul	0.00
85) Perylene-d12	23.57	264	990779	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	21756	6.59	ng/uL	0.00
5) Phenol-d5	6.91	99	101341	8.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	219925	29.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	276531	25.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.44	113	180479	17.91	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	158039	30.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.61	143	176449	30.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	326574	28.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	33645	3.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.79	166	1076598	33.66	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	1213176	30.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	27269m	5.38	ng/ul	0.00
57) Fluorene-d10	15.37	176	942019	33.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	133520	23.03	ng/ul	0.00
70) Anthracene-d10	17.23	188	1535893	34.28	ng/ul	0.00
78) Pyrene-d10	19.52	212	1730956	36.88	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.43	264	1990562	34.93	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.30	88	24302	7.001	ng/uL 96
6) Phenol	6.93	94	29741	2.456	ng/ul 99
44) Dimethylphthalate	13.84	163	49184	1.652	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
Data File : BM021423.D
Acq On : 11 Jul 2019 02:00
Operator : HP/JU
Sample : K3717-09
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF4A3

Quant Time: Jul 11 04:52:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 08 17:45:45 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
7/11/2019 5:23:35 PM

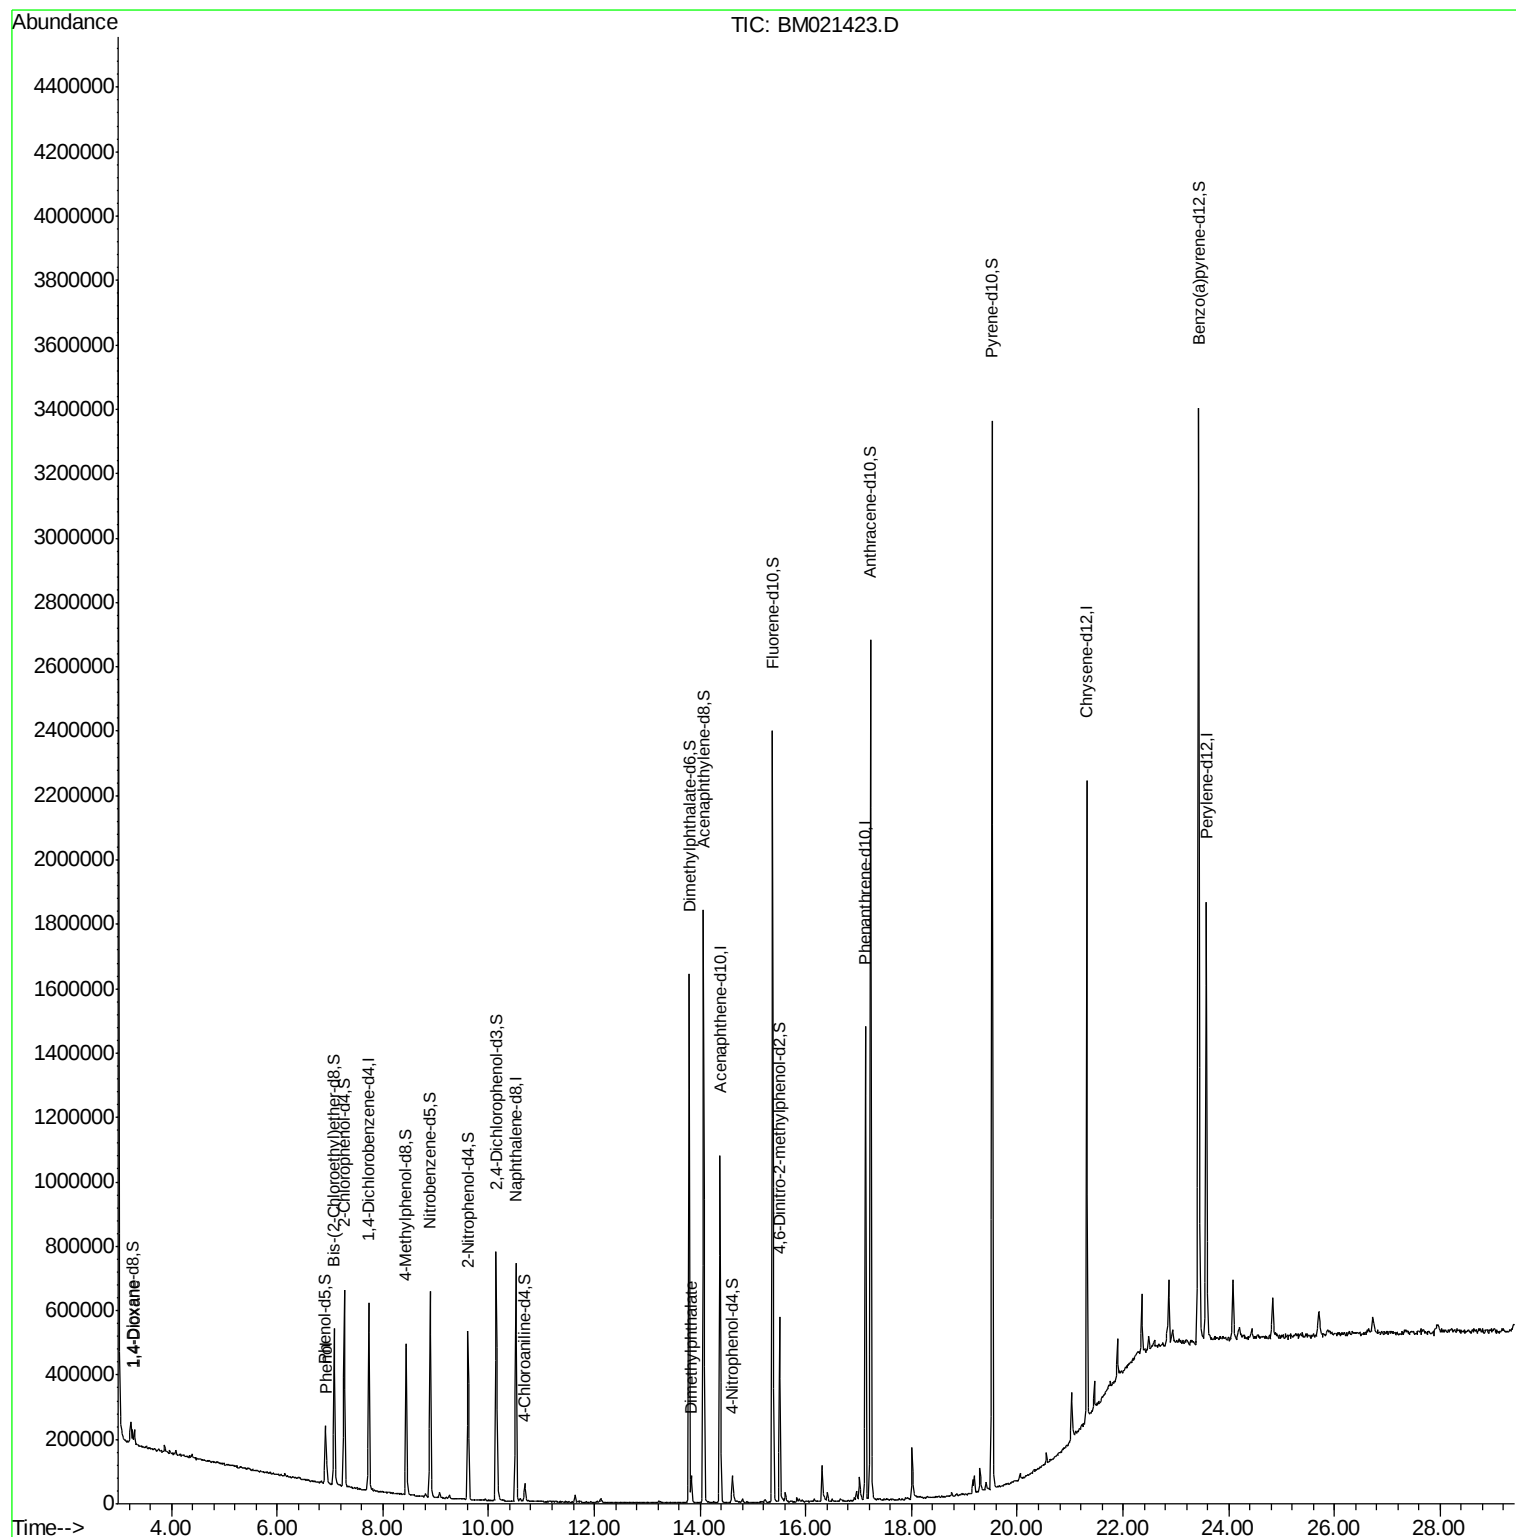

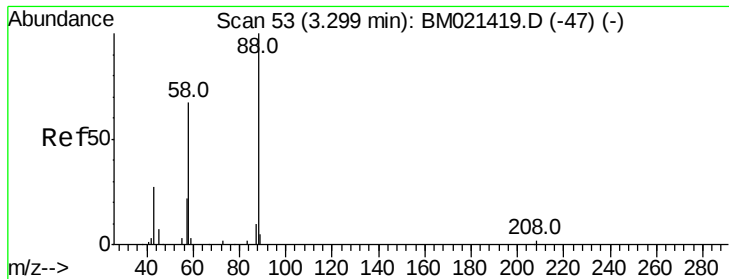

#2

1,4-Dioxane

Concen: 7.001 ng/uL

RT: 3.30 min Scan# 53

Delta R.T. -0.00 min

Lab File: BM021423.D

Acq: 11 Jul 2019 02:00

Instrument :

BNA_M





ClientSampleId :

BF4A3

Tot Ion:	88	Resp:	24302
Ion	Ratio	Lower	Upper
88	100		
43	28.8	23.4	35.2
58	67.8	50.6	75.8

Manual Integrations
APPROVED

mohammad
7/11/2019 5:23:35 PM

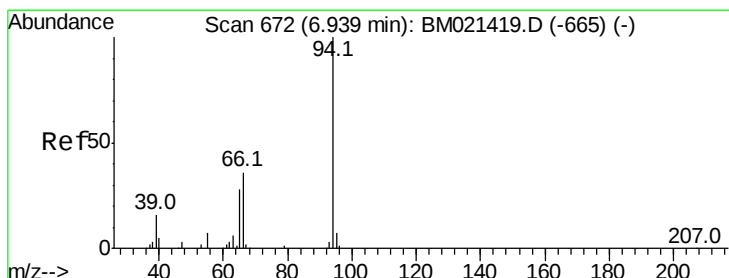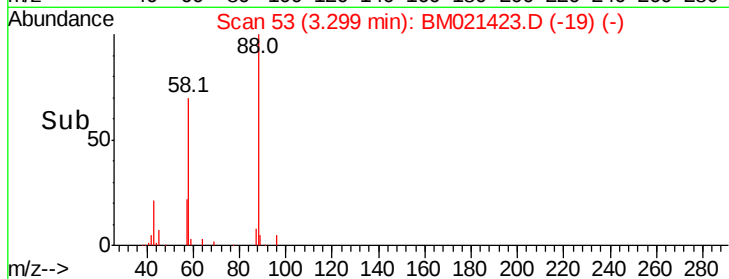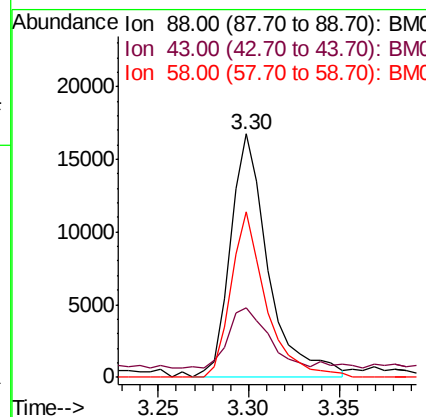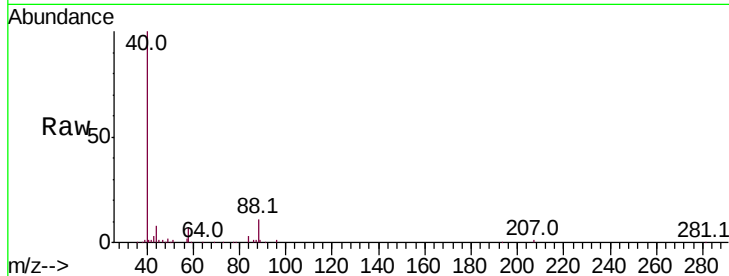

#6

Phenol

Concen: 2.456 ng/uL




RT: 6.93 min Scan# 671


Delta R.T. -0.01 min

Lab File: BM021423.D

Acq: 11 Jul 2019 02:00

Tgt Ion:	94	Resp:	29741
Ion	Ratio	Lower	Upper
94	100		
65	28.4	23.0	34.6
66	38.5	31.6	47.4

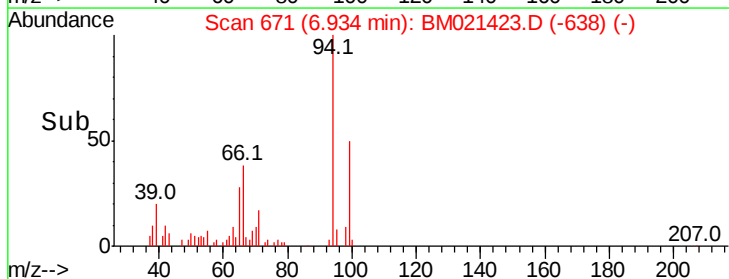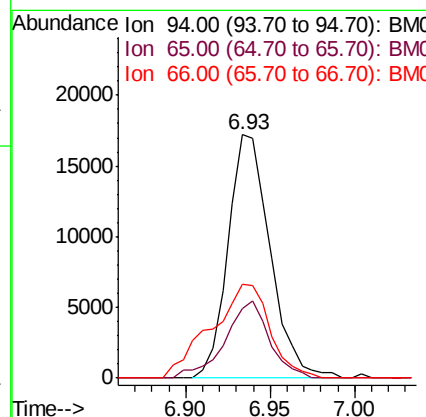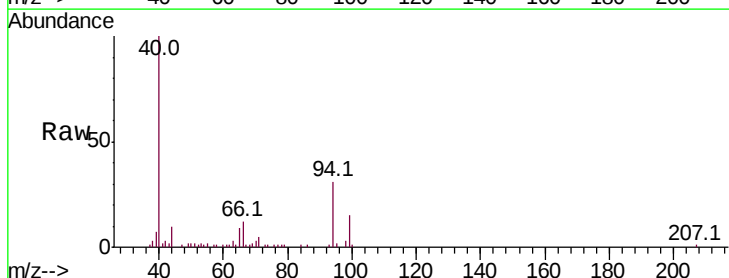

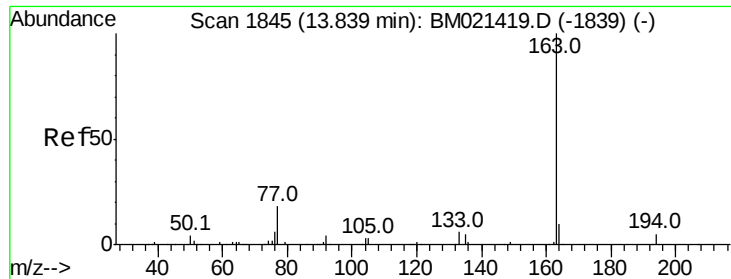

#44
 Dimethylphthalate
 Concen: 1.652 ng/ul
 RT: 13.84 min Scan# 1845
 Delta R.T. -0.00 min
 Lab File: BM021423.D
 Acq: 11 Jul 2019 02:00

Instrument :
 BNA_M
 ClientSampleId :
 BF4A3

Tot Ion:	163	Resp:	49184
Ion Ratio	Lower	Upper	
163	100		
194	4.9	3.6	5.4
164	11.0	8.3	12.5

Manual Integrations
 APPROVED

mohammad
 7/11/2019 5:23:35 PM

