

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
 Data File : BM021414.D
 Acq On : 10 Jul 2019 19:16
 Operator : HP/JU
 Sample : K3717-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF4A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	45	rBV	99756	128736	2.80%	0.354%
2	6.910	662	667	679	rVB	132747	233585	5.08%	0.643%
3	7.081	690	696	708	rVB	404011	665751	14.49%	1.833%
4	7.269	722	728	741	rVB	507609	804528	17.51%	2.215%
5	7.734	801	807	815	rVB	528584	844595	18.38%	2.325%
6	8.445	922	928	940	rVB	359481	596906	12.99%	1.643%
7	8.898	998	1005	1015	rBV	534553	902457	19.64%	2.485%
8	9.075	1032	1035	1041	rVB3	10238	17158	0.37%	0.047%
9	9.257	1064	1066	1075	rVB4	6642	11464	0.25%	0.032%
10	9.616	1120	1127	1138	rVB	427267	725597	15.79%	1.998%
11	10.151	1211	1218	1239	rVB	585546	1114578	24.26%	3.069%
12	10.522	1273	1281	1291	rVB	672127	1137225	24.75%	3.131%
13	10.686	1301	1309	1319	rBV2	43695	88779	1.93%	0.244%
14	11.639	1467	1471	1477	rVB3	9891	17244	0.38%	0.047%
15	12.128	1549	1554	1561	rVB4	7754	15282	0.33%	0.042%
16	13.792	1831	1837	1842	rBV	1331999	1860696	40.49%	5.123%
17	13.839	1842	1845	1855	rVB	99664	139307	3.03%	0.384%
18	14.074	1878	1885	1899	rBV	1422314	2167021	47.16%	5.966%
19	14.380	1930	1937	1946	rBV2	1000144	1523965	33.16%	4.196%
20	14.616	1969	1977	1990	rBV2	55134	129614	2.82%	0.357%
21	15.374	2099	2106	2119	rBV	1978929	2881375	62.70%	7.933%
22	15.510	2123	2129	2143	rVV	546455	773606	16.84%	2.130%
23	15.616	2143	2147	2153	rVB2	20213	29773	0.65%	0.082%
24	15.839	2179	2185	2187	rBV3	5212	6496	0.14%	0.018%
25	15.874	2187	2191	2197	rVB3	6920	11624	0.25%	0.032%
26	16.163	2236	2240	2244	rVB4	6344	8301	0.18%	0.023%
27	16.316	2259	2266	2272	rBV	29361	48547	1.06%	0.134%
28	16.416	2280	2283	2285	rBV	6857	7598	0.17%	0.021%
29	16.657	2319	2324	2327	rBV4	3613	5428	0.12%	0.015%
30	16.921	2364	2369	2372	rVV2	5823	9915	0.22%	0.027%
31	16.957	2372	2375	2381	rVV4	10141	16416	0.36%	0.045%
32	17.021	2381	2386	2394	rVV	30816	56490	1.23%	0.156%
33	17.127	2398	2404	2415	rVV2	1315431	1919557	41.77%	5.285%
34	17.227	2415	2421	2439	rVV	2439635	3459959	75.30%	9.526%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
 Data File : BM021414.D
 Acq On : 10 Jul 2019 19:16
 Operator : HP/JU
 Sample : K3717-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF4A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

35	17.898	2531	2535	2537	rBV4	4645	6476	0.14%	0.018%
36	18.015	2551	2555	2564	rBV2	75154	108544	2.36%	0.299%
37	19.074	2733	2735	2741	rVB4	8045	10267	0.22%	0.028%
38	19.157	2746	2749	2751	rBV	28368	33866	0.74%	0.093%
39	19.192	2751	2755	2759	rVB	68520	92741	2.02%	0.255%
40	19.304	2770	2774	2781	rBV6	28192	41020	0.89%	0.113%
41	19.415	2789	2793	2796	rBV	19962	28543	0.62%	0.079%
42	19.527	2806	2812	2828	rBV	3087247	4316496	93.94%	11.884%
43	21.027	3064	3067	3075	rVB6	54924	91199	1.98%	0.251%
44	21.315	3111	3116	3125	rBV	1770551	2278054	49.58%	6.272%
45	23.433	3470	3476	3490	rVB	2432091	4595165	100.00%	12.652%
46	23.580	3495	3501	3516	rVB	1231149	2358525	51.33%	6.494%


Sum of corrected areas: 36320469

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
Data File : BM021414.D
Acq On : 10 Jul 2019 19:16
Operator : HP/JU
Sample : K3717-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF4A7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

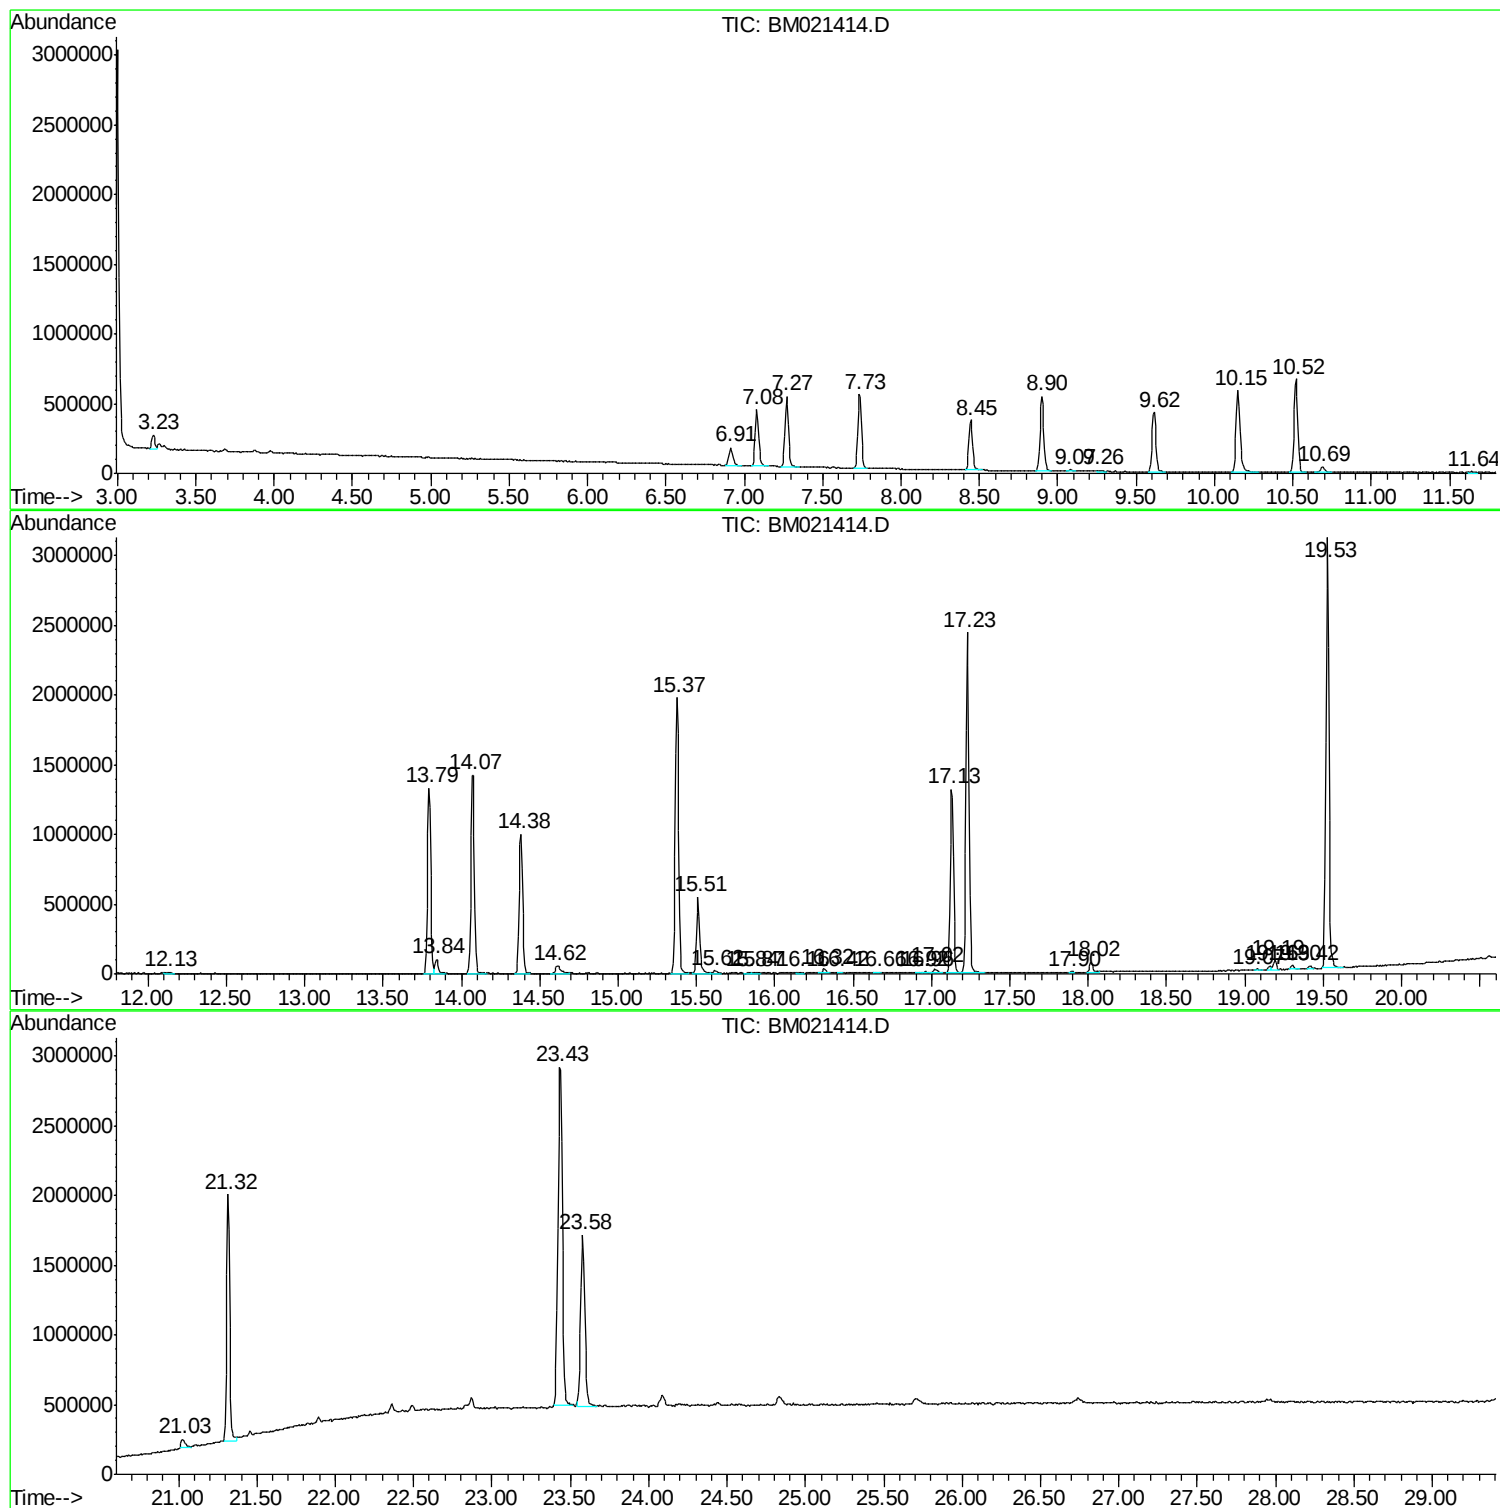

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071019\
Data File : BM021414.D
Acq On : 10 Jul 2019 19:16
Operator : HP/JU
Sample : K3717-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF4A7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071019\
Data File : BM021414.D
Acq On : 10 Jul 2019 19:16
Operator : HP/JU
Sample : K3717-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF4A7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc