

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
 Data File : BM021415.D
 Acq On : 10 Jul 2019 19:53
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF4A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.910	662	667	678	rVB	111636	212026	5.53%	0.617%
2	7.081	690	696	710	rVB	381167	621711	16.22%	1.808%
3	7.269	722	728	736	rBV	447843	724303	18.90%	2.107%
4	7.734	801	807	815	rVB	596636	931436	24.30%	2.709%
5	8.446	922	928	934	rBV	321630	529638	13.82%	1.541%
6	8.499	934	937	944	rVB3	25387	46042	1.20%	0.134%
7	8.563	946	948	953	rVB3	6479	7781	0.20%	0.023%
8	8.899	998	1005	1015	rBV	499206	831979	21.71%	2.420%
9	8.981	1017	1019	1024	rVB4	5334	6799	0.18%	0.020%
10	9.610	1119	1126	1137	rBV	404260	677829	17.68%	1.972%
11	9.869	1168	1170	1175	rBV2	2968	4246	0.11%	0.012%
12	10.151	1211	1218	1228	rBV	570765	1054609	27.51%	3.067%
13	10.522	1274	1281	1288	rBV	766778	1273508	33.22%	3.704%
14	10.687	1303	1309	1318	rBV	28877	71632	1.87%	0.208%
15	11.240	1399	1403	1408	rVB5	7712	14492	0.38%	0.042%
16	12.116	1546	1552	1560	rBV4	7855	14630	0.38%	0.043%
17	13.345	1755	1761	1762	rBV4	3554	4715	0.12%	0.014%
18	13.792	1831	1837	1842	rBV	1273520	1784916	46.57%	5.192%
19	13.839	1842	1845	1851	rVB	118709	161494	4.21%	0.470%
20	14.069	1874	1884	1896	rBV2	1417416	2095546	54.67%	6.095%
21	14.381	1930	1937	1952	rVB2	1160920	1740790	45.42%	5.063%
22	14.616	1971	1977	1988	rBV2	60708	128301	3.35%	0.373%
23	14.798	2003	2008	2011	rBV4	4240	5765	0.15%	0.017%
24	15.175	2068	2072	2074	rVB3	3683	5170	0.13%	0.015%
25	15.216	2074	2079	2083	rVB4	2750	4087	0.11%	0.012%
26	15.375	2099	2106	2118	rBV	1997789	2793047	72.87%	8.124%
27	15.510	2123	2129	2141	rVV	487973	664328	17.33%	1.932%
28	15.616	2141	2147	2152	rVB3	21067	32907	0.86%	0.096%
29	15.963	2202	2206	2209	rBV4	2977	4057	0.11%	0.012%
30	16.092	2223	2228	2229	rBV3	2846	4062	0.11%	0.012%
31	16.157	2235	2239	2244	rBV5	7109	8498	0.22%	0.025%
32	16.528	2298	2302	2307	rBV5	4383	7746	0.20%	0.023%
33	16.657	2319	2324	2332	rBV	19971	33069	0.86%	0.096%
34	16.886	2359	2363	2365	rBV3	2804	4419	0.12%	0.013%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
 Data File : BM021415.D
 Acq On : 10 Jul 2019 19:53
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF4A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

35	16.922	2365	2369	2373	rVV3	5145	8877	0.23%	0.026%
36	17.127	2398	2404	2415	rBV2	1479383	2113080	55.13%	6.146%
37	17.227	2415	2421	2430	rBV2	2174027	3036012	79.21%	8.831%
38	17.410	2450	2452	2456	rBV4	3564	6199	0.16%	0.018%
39	17.892	2528	2534	2538	rBV7	7503	12539	0.33%	0.036%
40	18.016	2550	2555	2566	rBV2	76018	120257	3.14%	0.350%
41	18.145	2575	2577	2581	rVB4	6104	6090	0.16%	0.018%
42	18.486	2633	2635	2639	rBV5	4670	5809	0.15%	0.017%
43	18.769	2680	2683	2688	rBV5	4984	8728	0.23%	0.025%
44	19.098	2735	2739	2740	rBV4	4698	6719	0.18%	0.020%
45	19.163	2746	2750	2757	rBV	22481	36344	0.95%	0.106%
46	19.239	2761	2763	2766	rBV4	4697	4929	0.13%	0.014%
47	19.304	2771	2774	2777	rBV4	23256	25757	0.67%	0.075%
48	19.416	2790	2793	2797	rVB	16415	18792	0.49%	0.055%
49	19.527	2806	2812	2824	rBV	2719122	3656676	95.40%	10.636%
50	21.027	3064	3067	3072	rBV4	55393	89234	2.33%	0.260%
51	21.315	3111	3116	3125	rBV	1753862	2448796	63.89%	7.123%
52	23.439	3470	3477	3487	rVB	2023496	3832982	100.00%	11.149%
53	23.580	3495	3501	3511	rVB	1264004	2436745	63.57%	7.088%


Sum of corrected areas: 34380143

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071019\
Data File : BM021415.D
Acq On : 10 Jul 2019 19:53
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF4A8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

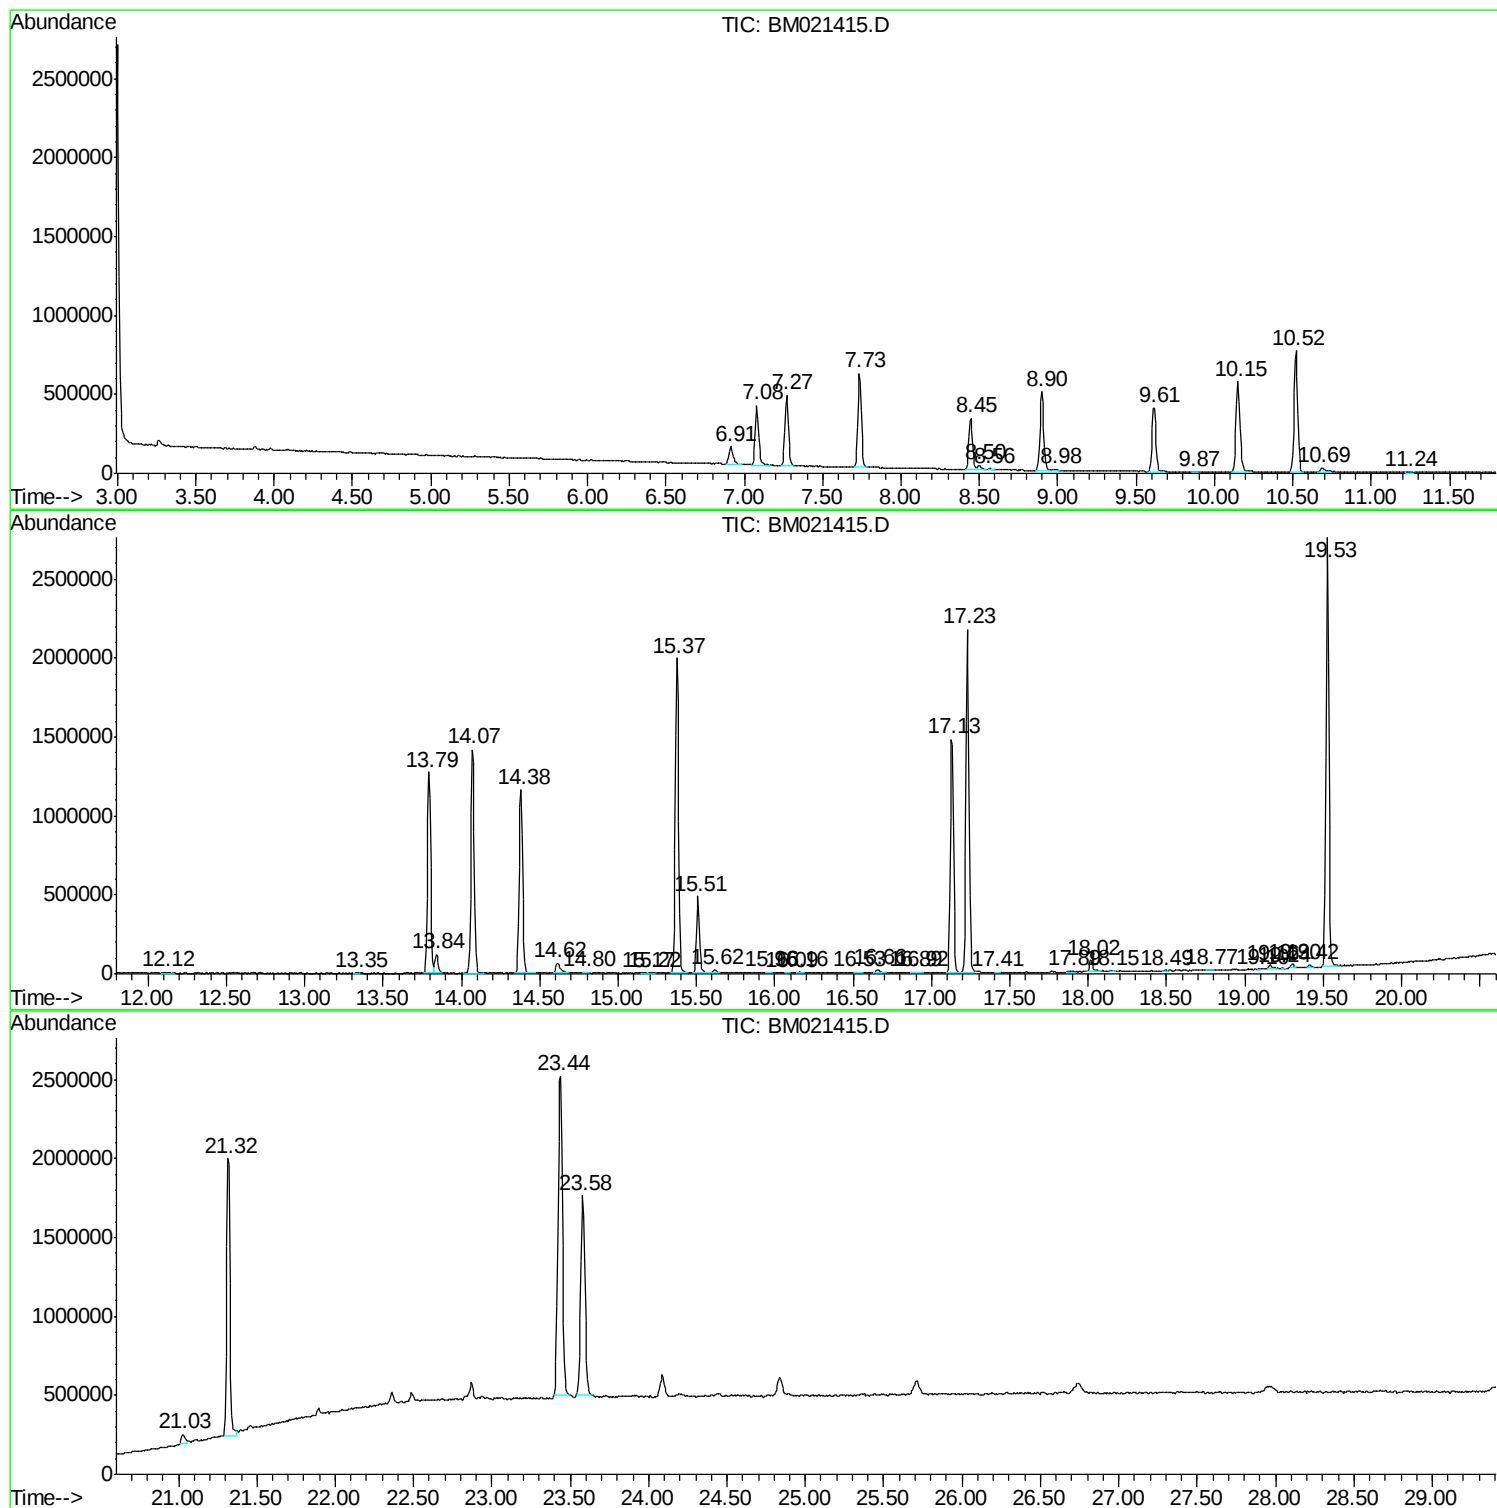

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071019\
Data File : BM021415.D
Acq On : 10 Jul 2019 19:53
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF4A8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071019\
Data File : BM021415.D
Acq On : 10 Jul 2019 19:53
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF4A8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc