

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040791.D
 Acq On : 10 Jul 2023 09:26
 Operator : MA/JU
 Sample : PB153949BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 11 03:55:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3777	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	13437	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.527	164	6284	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.278	188	11219	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	6242	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.88
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	33740	5.687	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	5719	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	6388	0.319	ng/ul	0.00
Target Compounds						
20) Pyrene	19.673	202	1308	0.046	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
Data File : BM040791.D
Acq On : 10 Jul 2023 09:26
Operator : MA/JU
Sample : PB153949BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jul 11 03:55:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

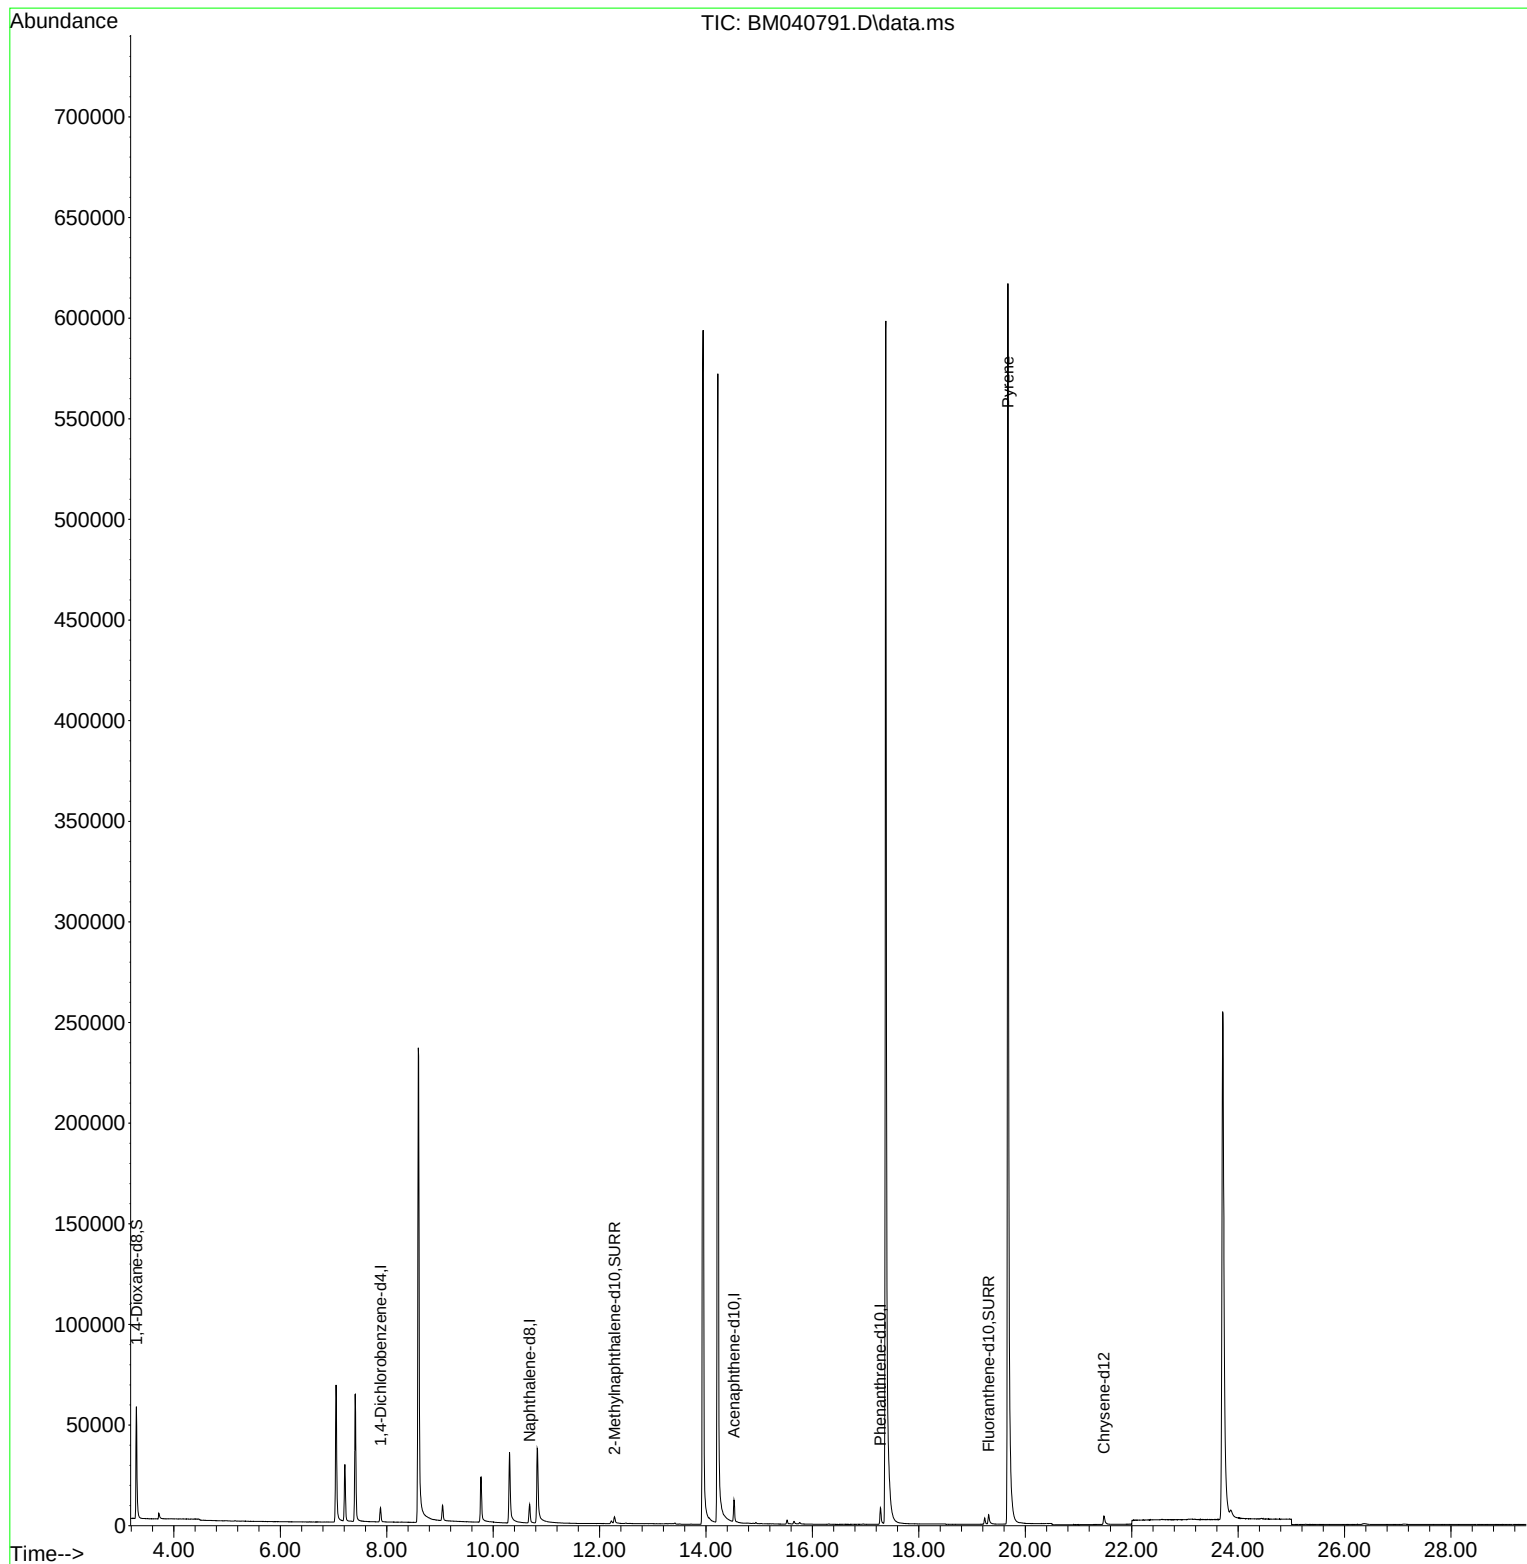

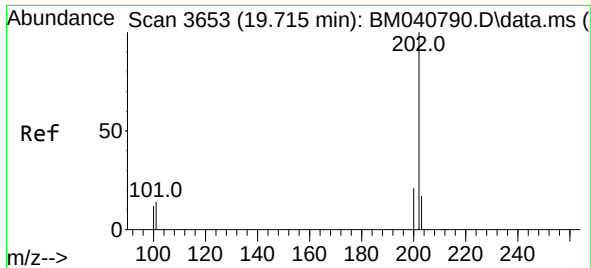

#20
 Pyrene
 Concen: 0.046 ng/ul
 RT: 19.673 min Scan# 30
 Delta R.T. -0.042 min
 Lab File: BM040791.D
 Acq: 10 Jul 2023 09:26

Instrument :
 BNA_M
 ClientSampleId :

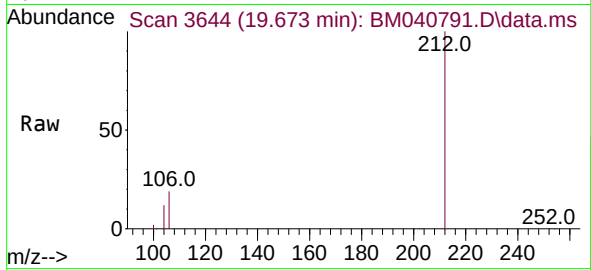

Tgt Ion:202 Resp: 1308
 Ion Ratio Lower Upper
 202 100
 101 195.4 12.6 18.8#
 100 1486.4 9.8 14.6#

