

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040797.D
 Acq On : 10 Jul 2023 13:09
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 11 03:56:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3020	0.400	ng/ul	0.00
4) Naphthalene-d8	10.685	136	10997	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.527	164	5092	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.278	188	9066	0.400	ng/ul	-0.01
17) Chrysene-d12	21.474	240	5360	0.400	ng/ul	-0.01
23) Perylene-d12	23.860	264	5319	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	22023	4.642	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	4446	0.288	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	5560	0.324	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.330	88	12535	2.596	ng/ul	89
20) Pyrene	19.673	202	1199	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.710	252	1770	0.095	ng/ul#	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
Data File : BM040797.D
Acq On : 10 Jul 2023 13:09
Operator : MA/JU
Sample : 03404-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jul 11 03:56:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

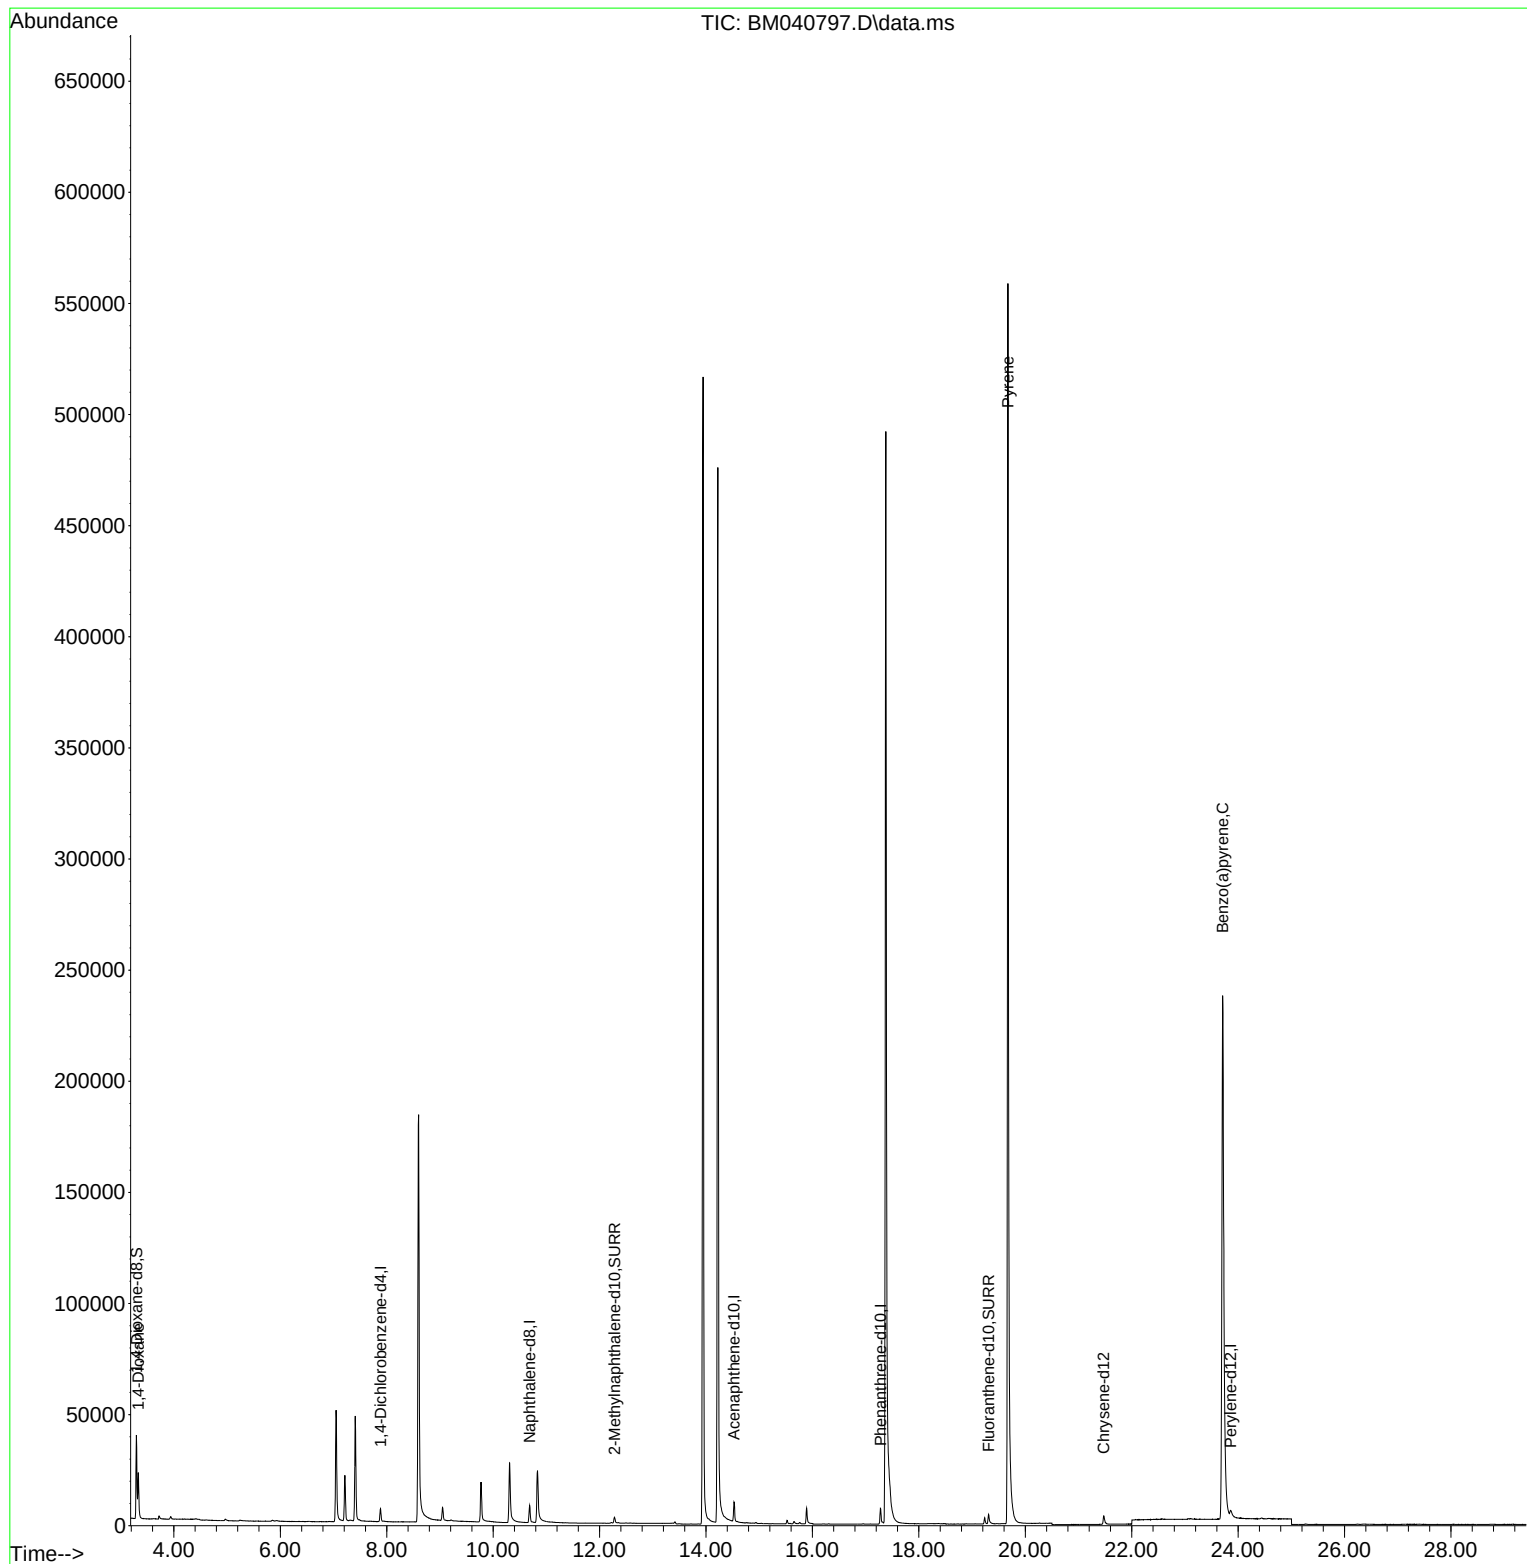



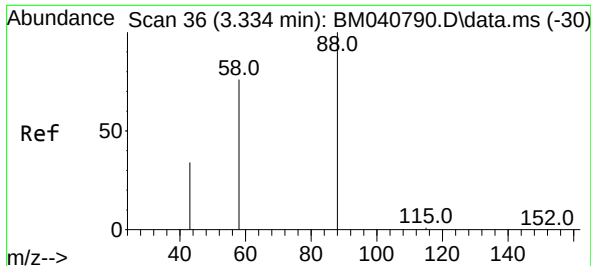


#2
1,4-Dioxane
Concen: 2.596 ng/ul
RT: 3.330 min Scan# 31
Delta R.T. -0.004 min
Lab File: BM040797.D
Acq: 10 Jul 2023 13:09

Instrument :
BNA_M
ClientSampleId :



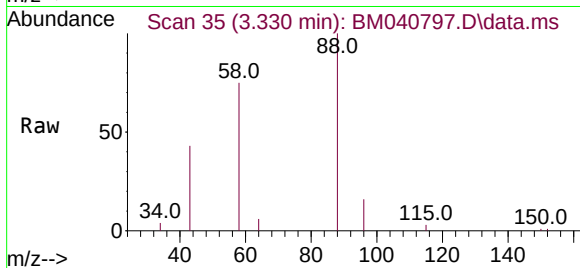



Tgt Ion: 88 Resp: 12535
Ion Ratio Lower Upper
88 100
43 42.7 36.1 54.1
58 74.6 49.8 74.8

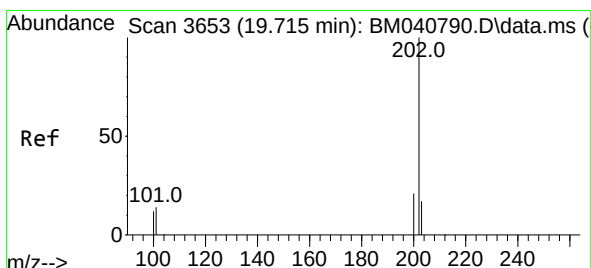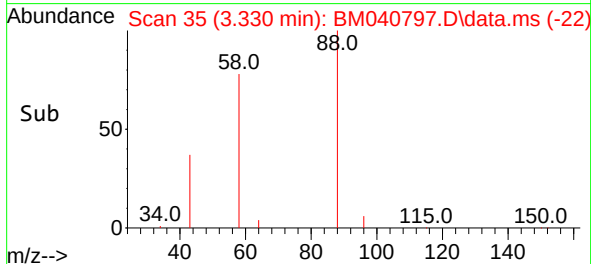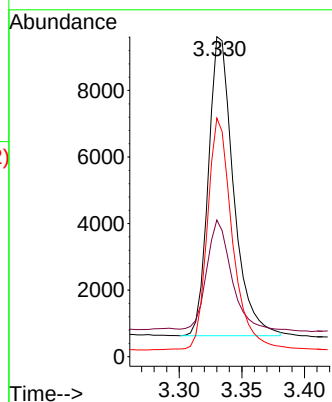

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.673 min Scan# 3644
Delta R.T. -0.042 min
Lab File: BM040797.D
Acq: 10 Jul 2023 13:09


Tgt Ion: 202 Resp: 1199
Ion Ratio Lower Upper
202 100
101 190.5 12.6 18.8#
100 1396.2 9.8 14.6#

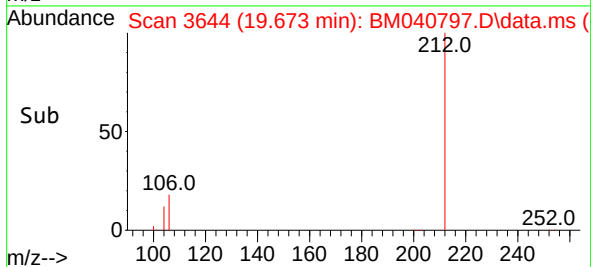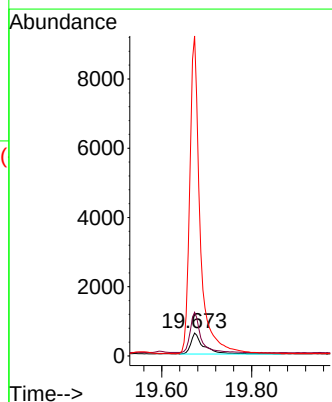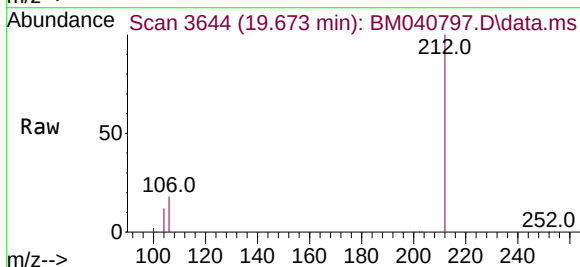

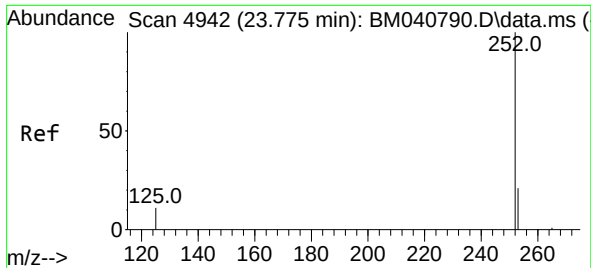

#26
 Benzo(a)pyrene
 Concen: 0.095 ng/ul
 RT: 23.710 min Scan# 4942
 Delta R.T. -0.064 min
 Lab File: BM040797.D
 Acq: 10 Jul 2023 13:09

Instrument :
 BNA_M
 ClientSampleId :

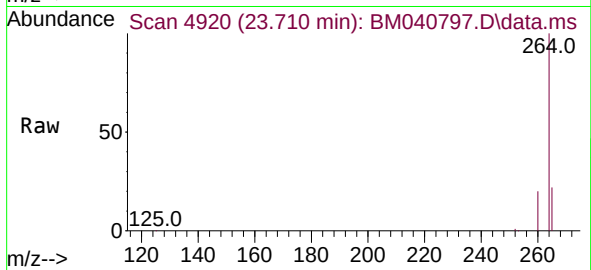

Tgt Ion:252 Resp: 1770
 Ion Ratio Lower Upper
 252 100
 253 66.9 22.9 34.3#
 125 86.8 21.0 31.4#

