

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040801.D
 Acq On : 10 Jul 2023 15:38
 Operator : MA/JU
 Sample : 03404-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 11 03:57:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3139	0.400	ng/ul	0.00
4) Naphthalene-d8	10.685	136	11701	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	5481	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	10147	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	6248	0.400	ng/ul	0.00
23) Perylene-d12	23.860	264	5875	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	17371	3.523	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	3512	0.214	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	5021	0.251	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.673	202	1073	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.713	252	1661	0.081	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
Data File : BM040801.D
Acq On : 10 Jul 2023 15:38
Operator : MA/JU
Sample : 03404-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 11 03:57:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration




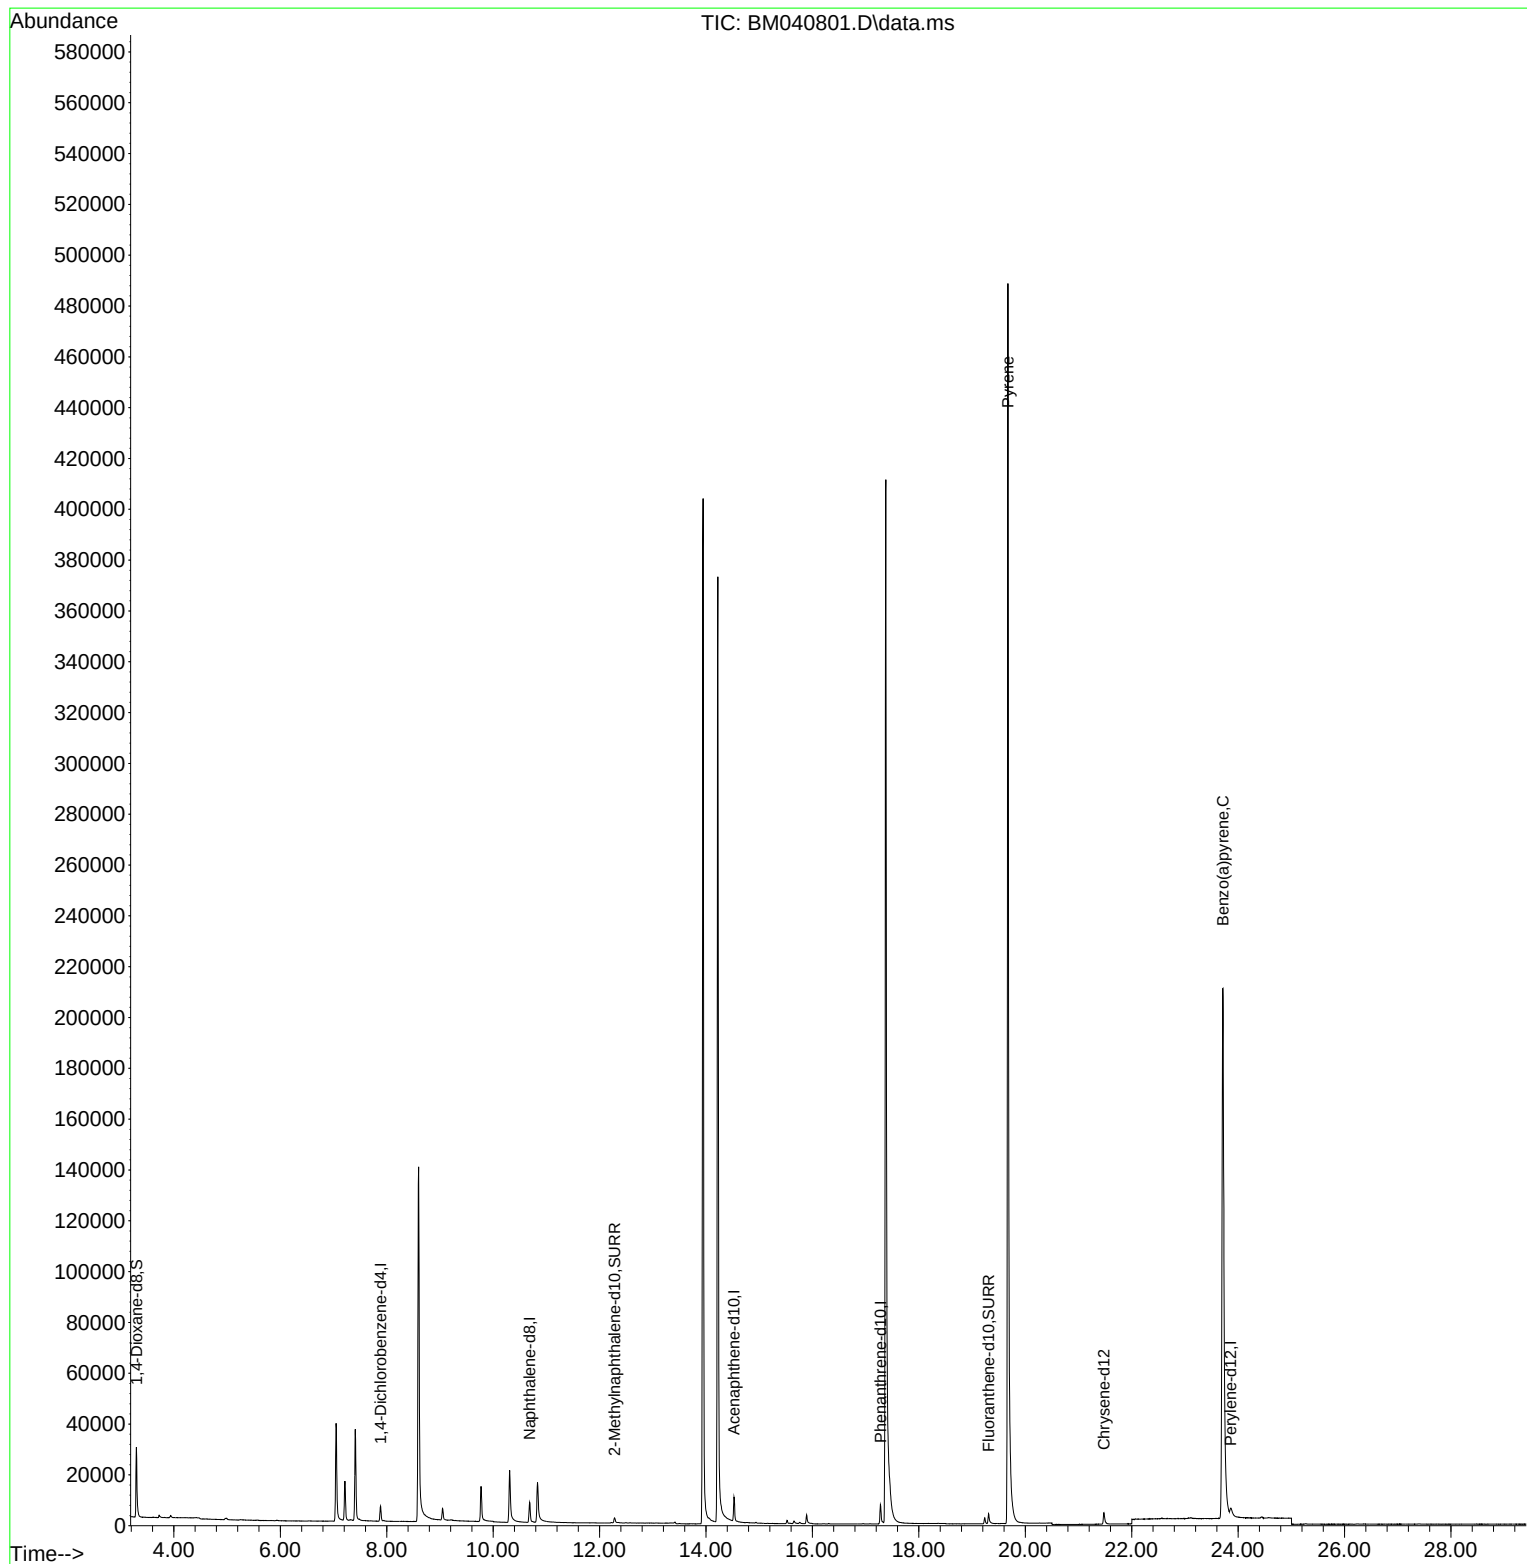


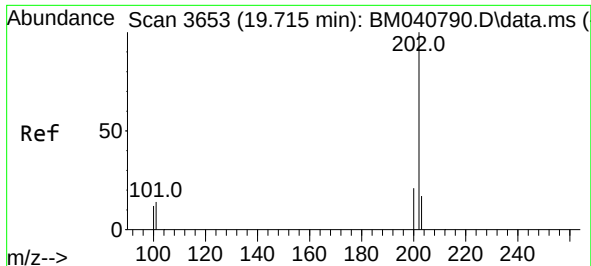

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.673 min Scan# 3644
Delta R.T. -0.042 min
Lab File: BM040801.D
Acq: 10 Jul 2023 15:38

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 1073
Ion Ratio Lower Upper
202 100
101 189.1 12.6 18.8#
100 1399.7 9.8 14.6#

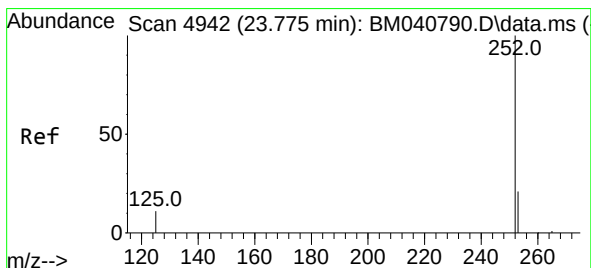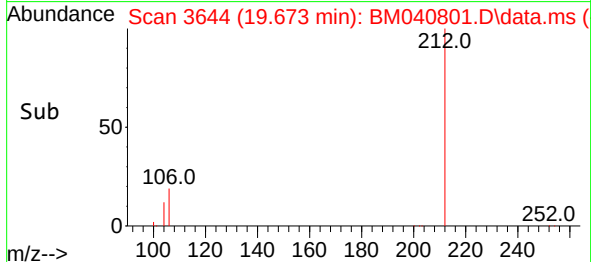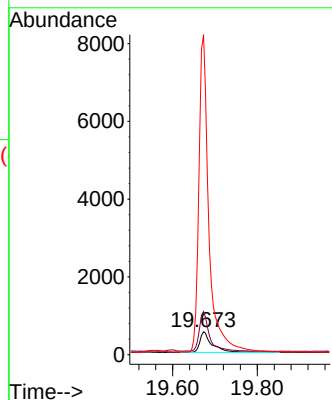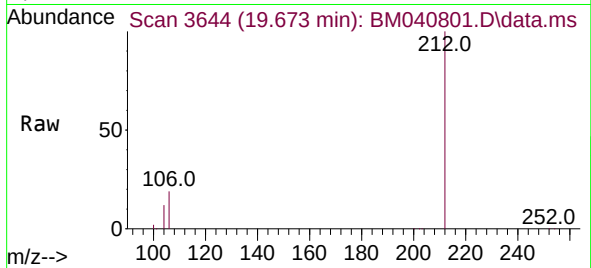

#26
Benzo(a)pyrene
Concen: 0.081 ng/ul
RT: 23.713 min Scan# 4921
Delta R.T. -0.061 min
Lab File: BM040801.D
Acq: 10 Jul 2023 15:38

Tgt Ion:252 Resp: 1661
Ion Ratio Lower Upper
252 100
253 68.7 22.9 34.3#
125 99.4 21.0 31.4#

