




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040791.D
 Acq On : 10 Jul 2023 09:26
 Operator : MA/JU
 Sample : PB153949BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK949

Manual IntegrationsAPPROVED

Quant Time: Jul 11 03:55:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

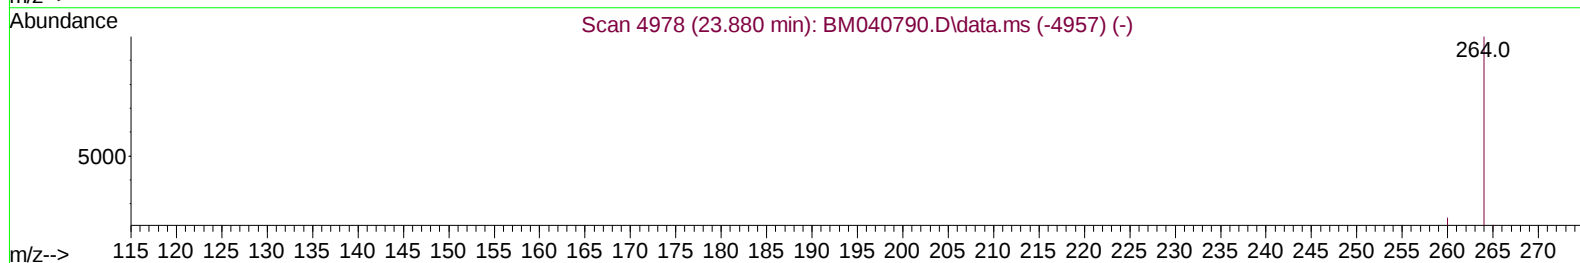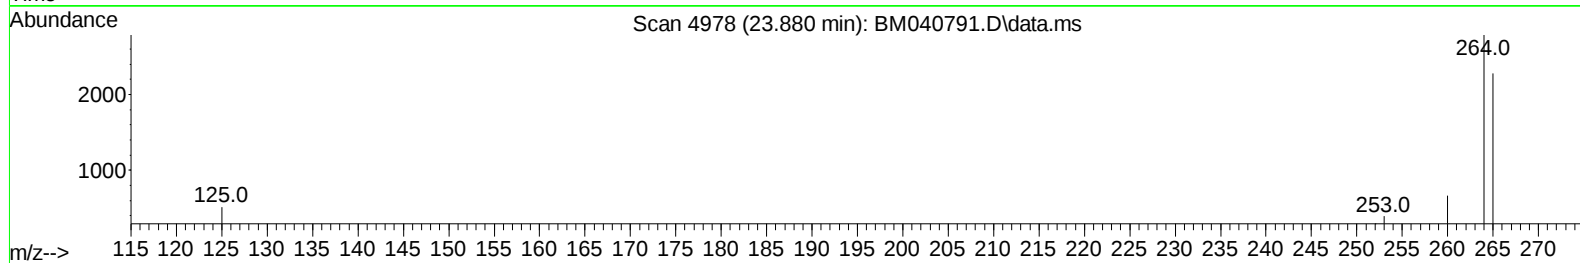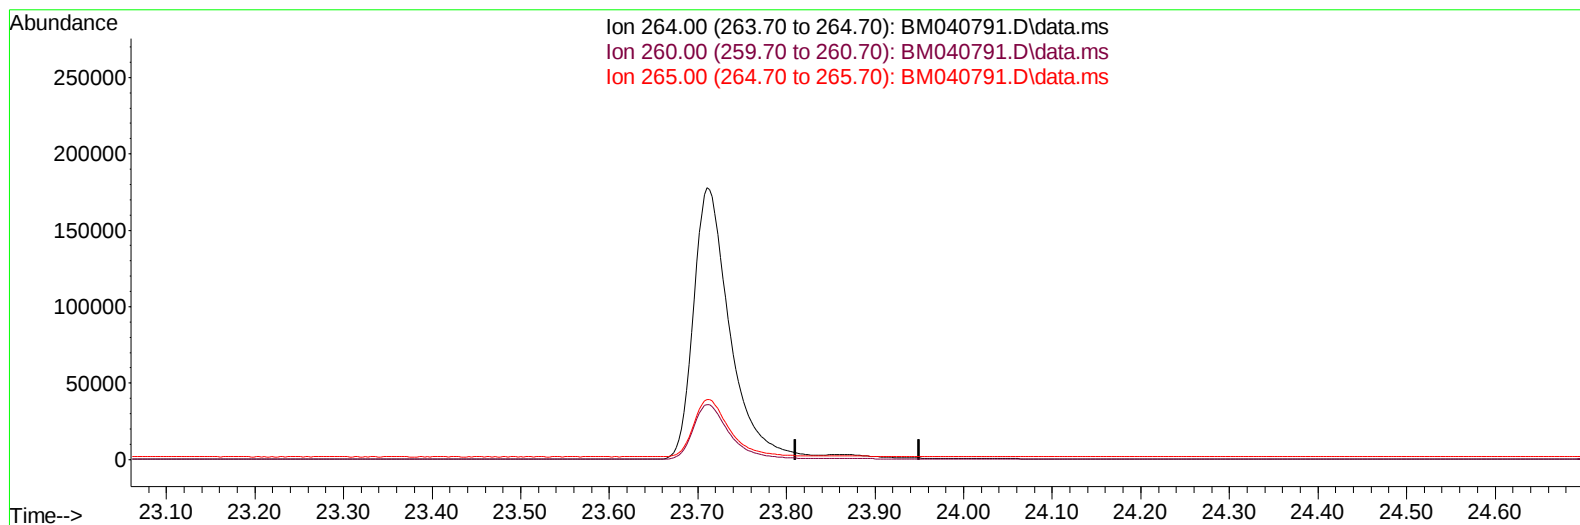

TIC: BM040791.D\data.ms

(23) Perylene-d12 (I)

23.880min (-23.880) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040791.D
 Acq On : 10 Jul 2023 09:26
 Operator : MA/JU
 Sample : PB153949BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK949

Manual IntegrationsAPPROVED

Quant Time: Jul 11 03:55:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

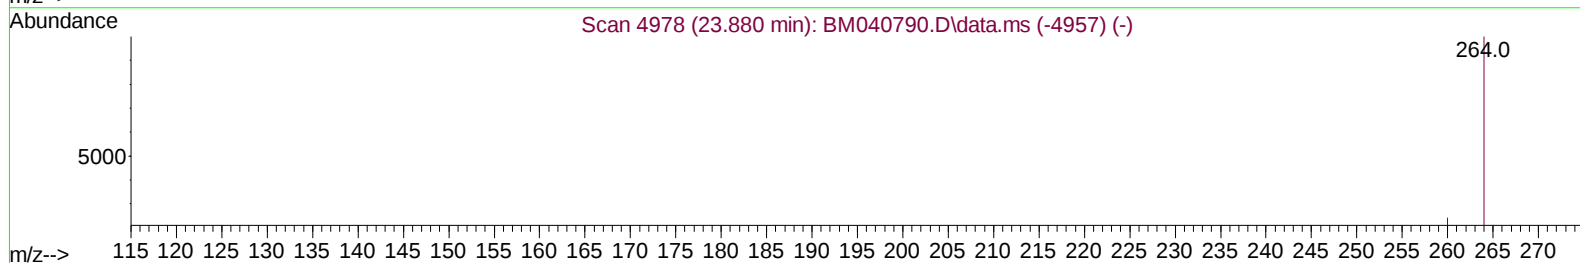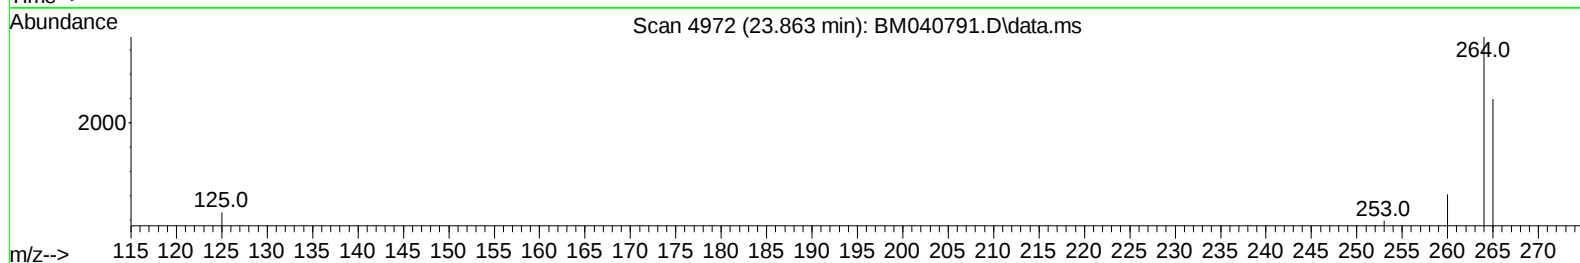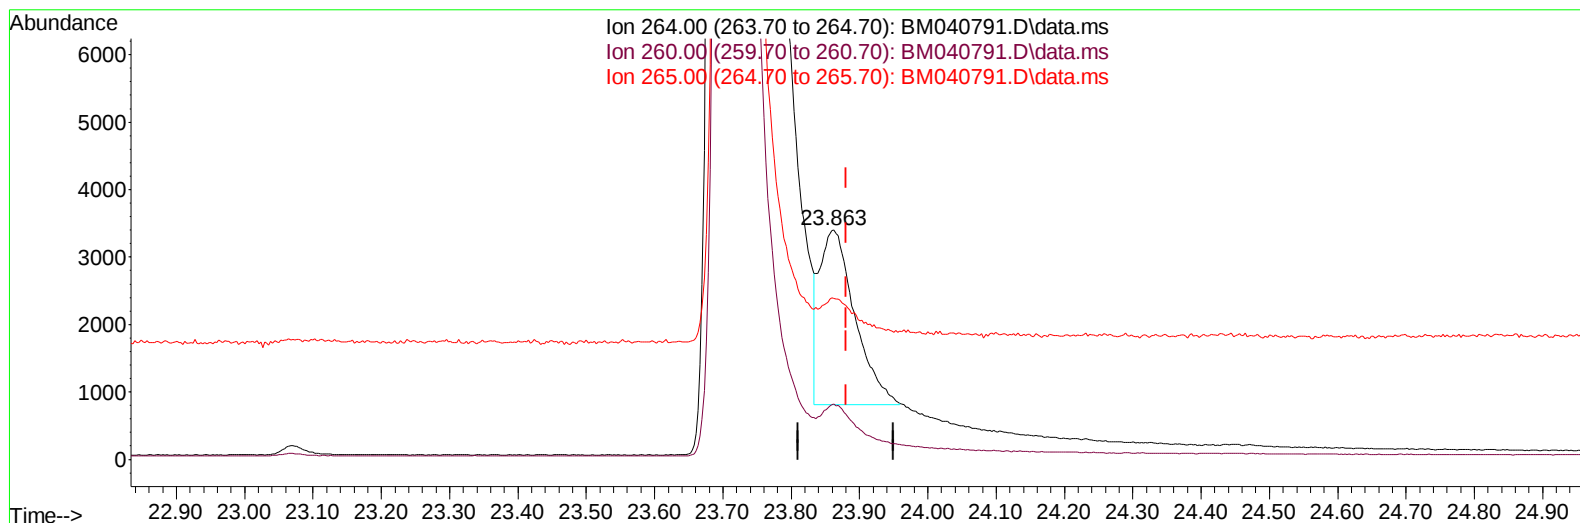

TIC: BM040791.D\data.ms

(23) Perylene-d12 (I)

23.863min (-0.017) 0.40 ng/ul m

response 9358

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	24.16
265.00	79.20	70.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040791.D
 Acq On : 10 Jul 2023 09:26
 Operator : MA/JU
 Sample : PB153949BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK949

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

Quant Time: Jul 11 03:55:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3777	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	13437	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	6284	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	11219	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	6242	0.400	ng/ul	0.00
23) Perylene-d12	23.863	264	9358m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	33740	5.687	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	5719	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	6388	0.319	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
Data File : BM040791.D
Acq On : 10 Jul 2023 09:26
Operator : MA/JU
Sample : PB153949BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK949

Manual IntegrationsAPPROVED

Quant Time: Jul 11 03:55:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

