

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040796.D
 Acq On : 10 Jul 2023 12:31
 Operator : MA/JU
 Sample : 03404-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBW45

Quant Time: Jul 11 03:56:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3123	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	11764	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	5613	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	10641	0.400	ng/ul	-0.01
17) Chrysene-d12	21.474	240	6895	0.400	ng/ul	-0.01
23) Perylene-d12	23.865	264	5835	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	14733	3.003	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	3395	0.206	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	4757	0.215	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.330	88	6229	1.247	ng/ul	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
Data File : BM040796.D
Acq On : 10 Jul 2023 12:31
Operator : MA/JU
Sample : 03404-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBW45

Quant Time: Jul 11 03:56:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

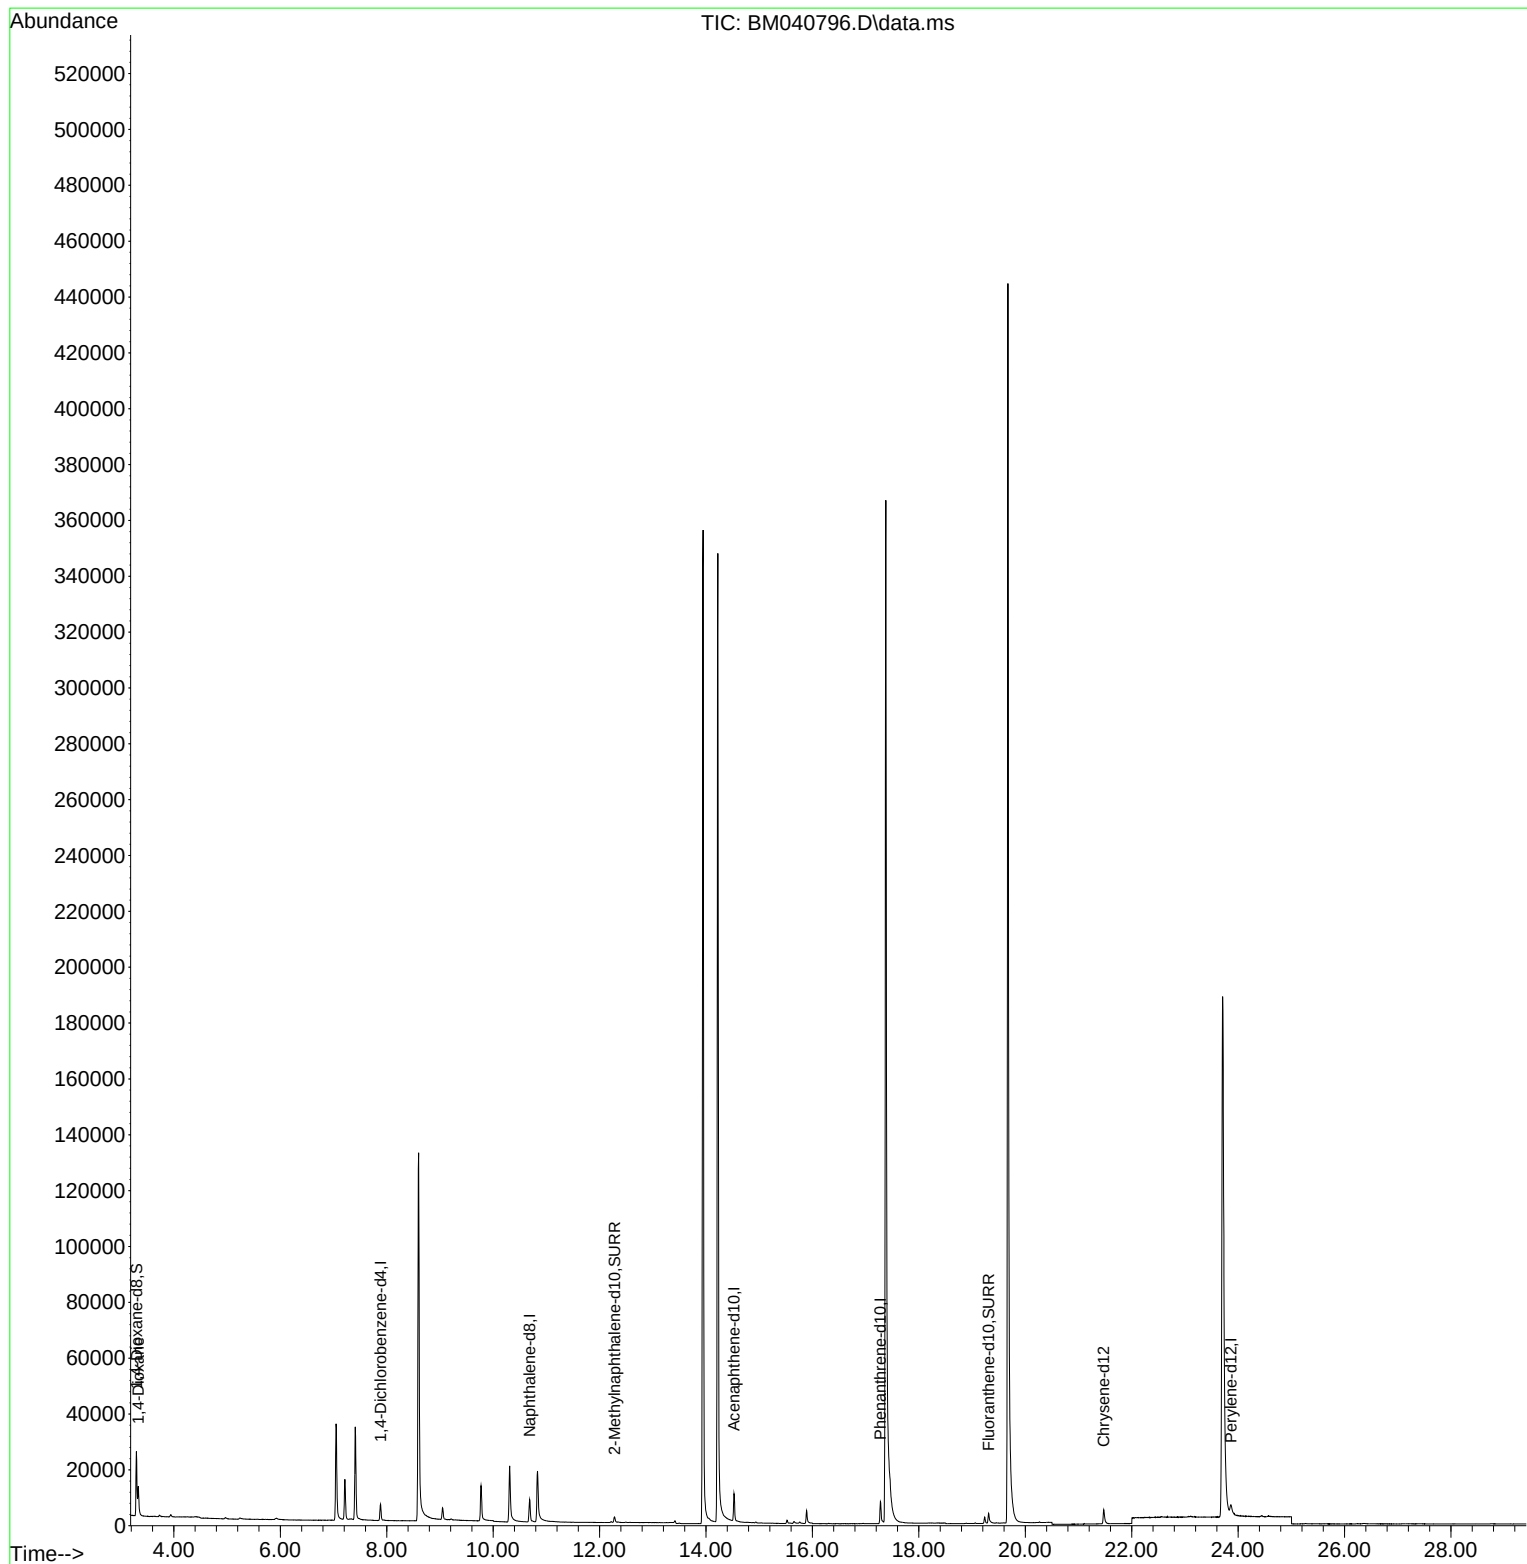

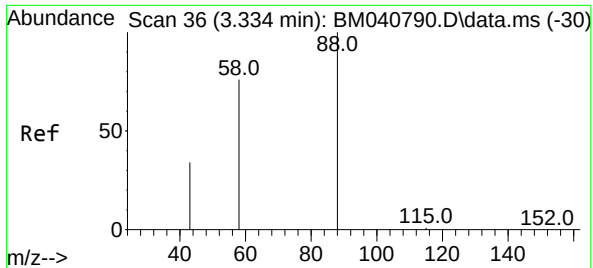

#2
 1,4-Dioxane
 Concen: 1.247 ng/ul
 RT: 3.330 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BM040796.D
 Acq: 10 Jul 2023 12:31

Instrument :
 BNA_M
 ClientSampleId :
 YBW45

Tgt Ion: 88 Resp: 6229

Ion	Ratio	Lower	Upper
88	100		
43	51.6	36.1	54.1
58	71.8	49.8	74.8

