

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
 Data File : BM040798.D
 Acq On : 10 Jul 2023 13:46
 Operator : MA/JU
 Sample : 03404-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBW47

Quant Time: Jul 11 03:56:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3388	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	12644	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	5836	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	10640	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	6261	0.400	ng/ul	0.00
23) Perylene-d12	23.862	264	6057	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	17951	3.373	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	3665	0.207	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	4596	0.229	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.334	88	1848	0.341	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071023\
Data File : BM040798.D
Acq On : 10 Jul 2023 13:46
Operator : MA/JU
Sample : 03404-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBW47

Quant Time: Jul 11 03:56:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

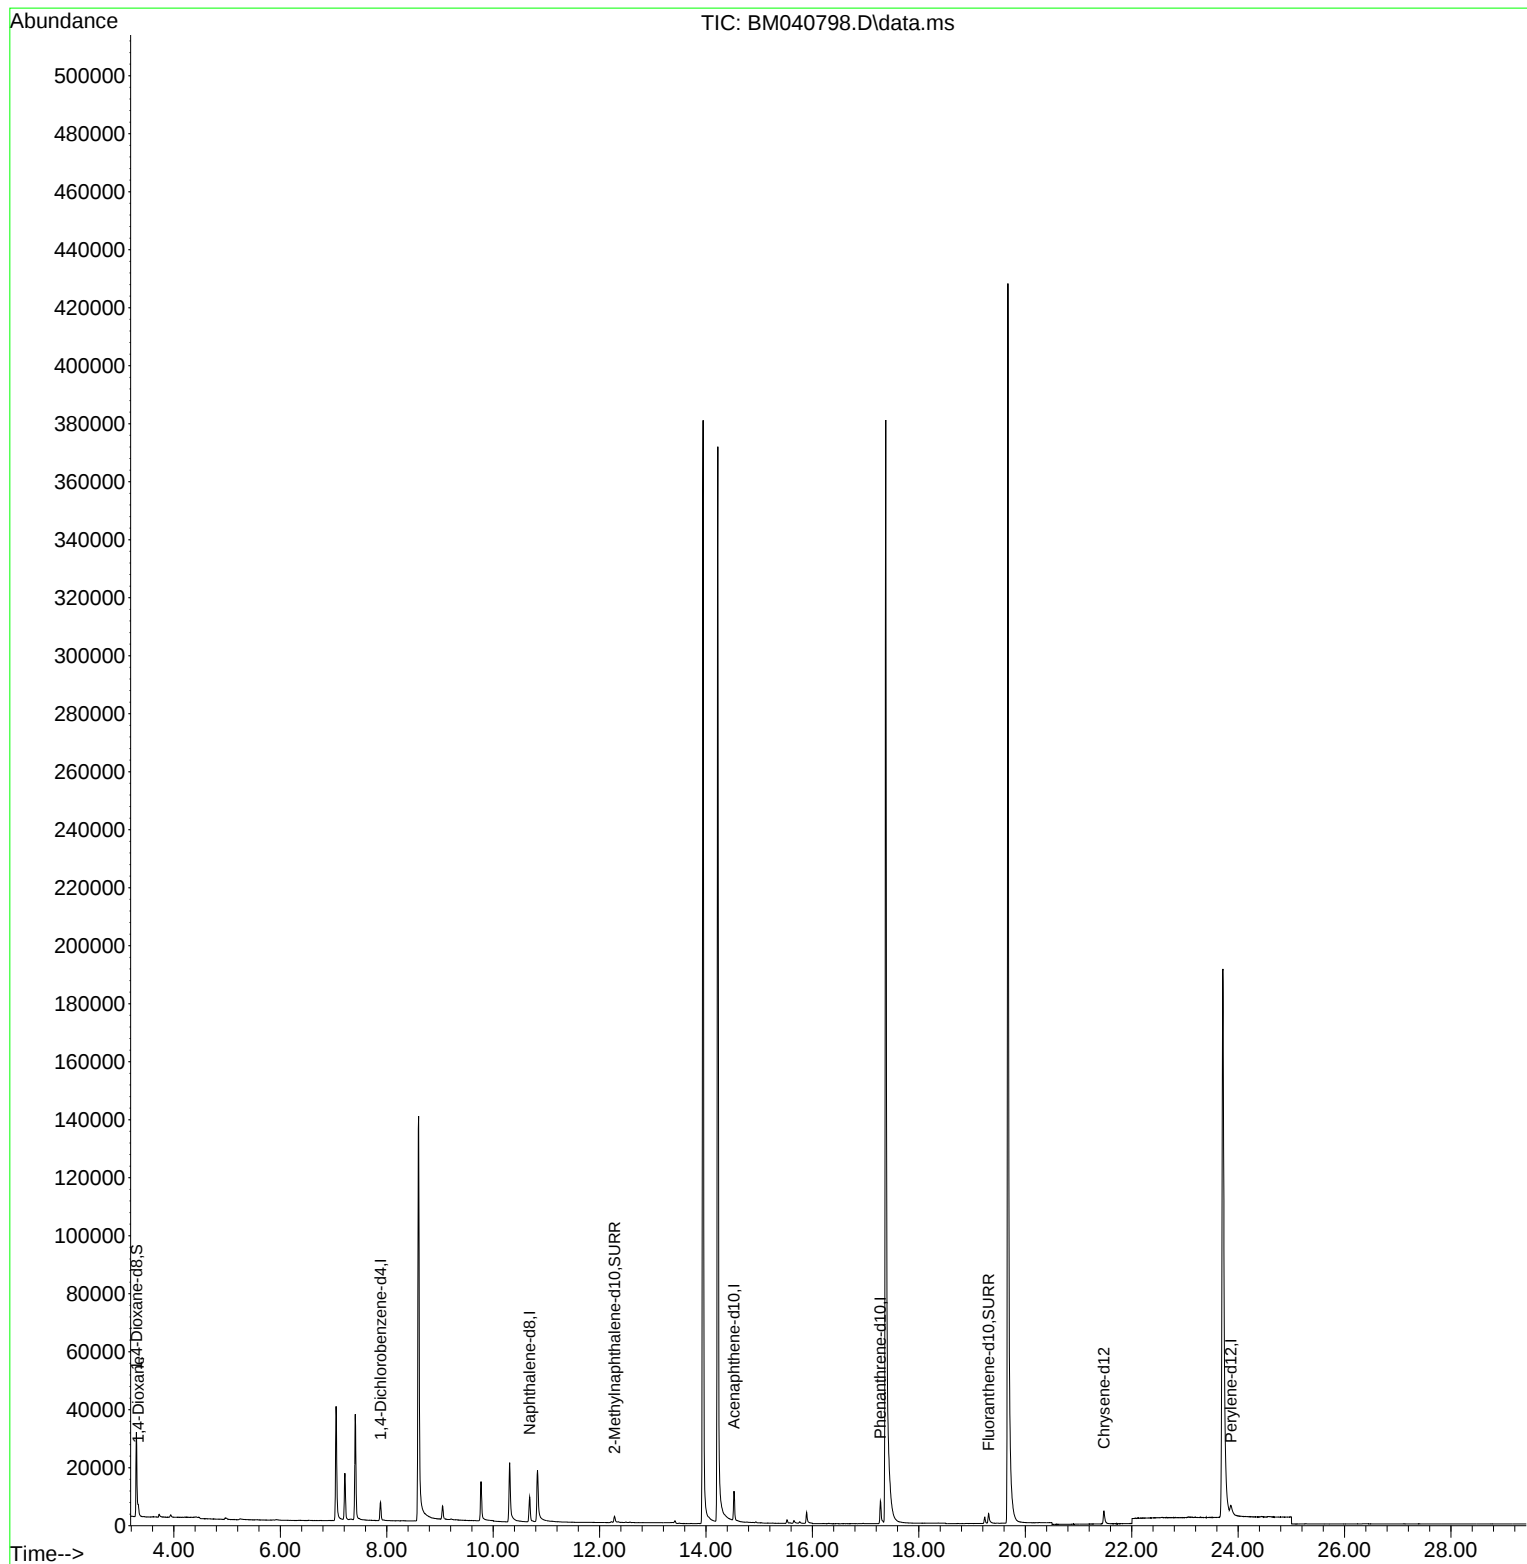

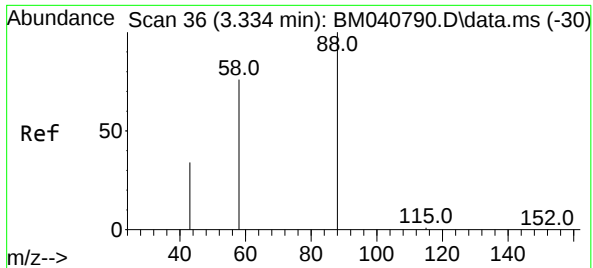

#2
 1,4-Dioxane
 Concen: 0.341 ng/ul
 RT: 3.334 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BM040798.D
 Acq: 10 Jul 2023 13:46

Instrument :
 BNA_M
 ClientSampleId :
 YBW47

Tgt Ion: 88 Resp: 1848

Ion	Ratio	Lower	Upper
88	100		
43	65.6	36.1	54.1#
58	59.9	49.8	74.8

