
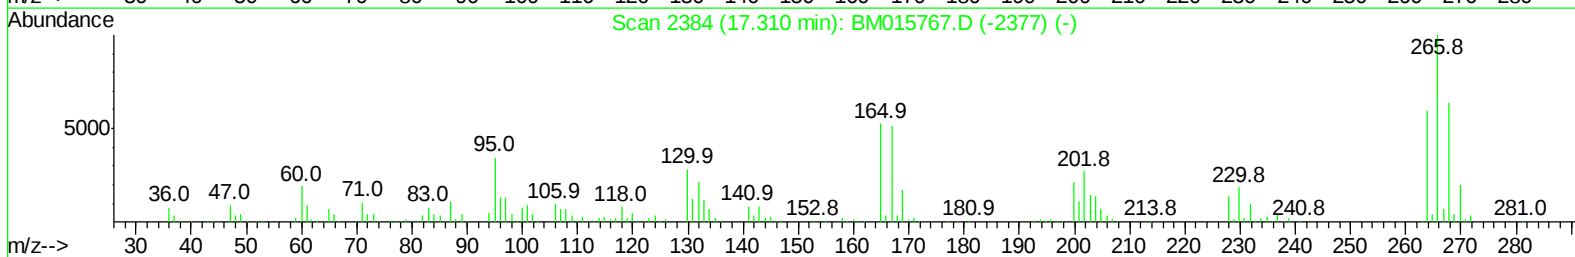
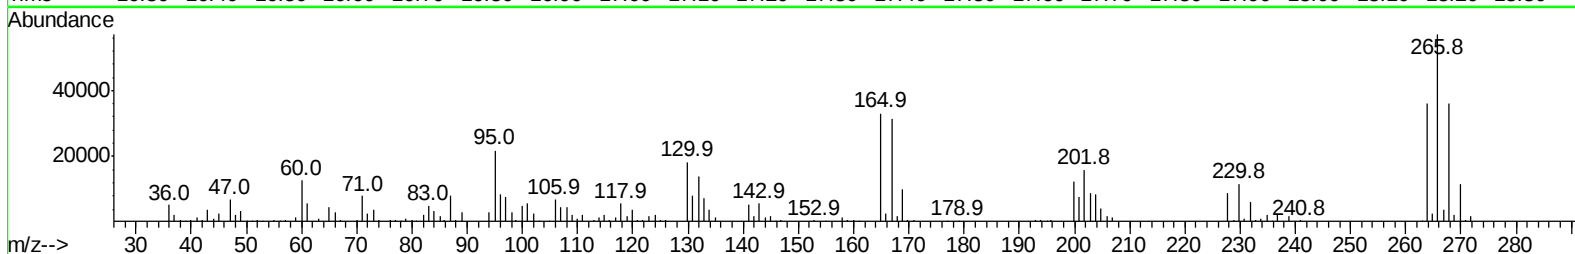


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071118\
Data File : BM015884.D
Acq On : 11 Jul 2018 12:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 09:19:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

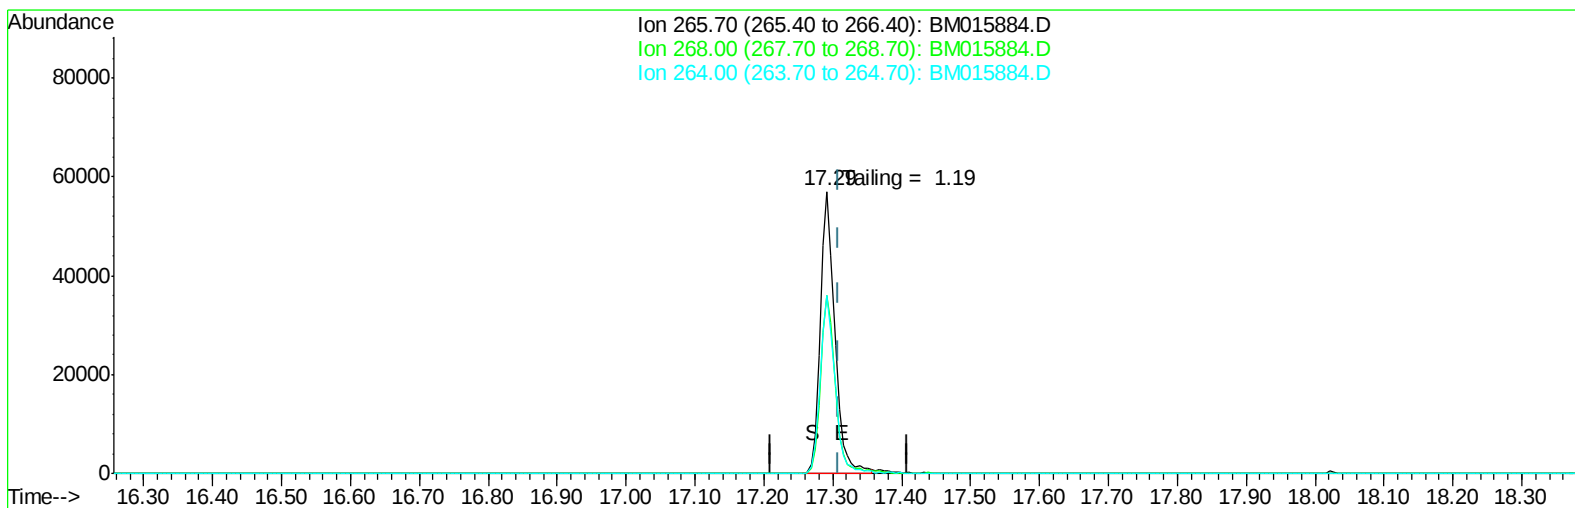

TIC: BM015884.D

(69) Pentachlorophenol (C)




17.292min (-0.018) 11200.36ng

response 84394

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.02
264.00	61.20	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071118\
Data File : BM015884.D
Acq On : 11 Jul 2018 12:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 09:19:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

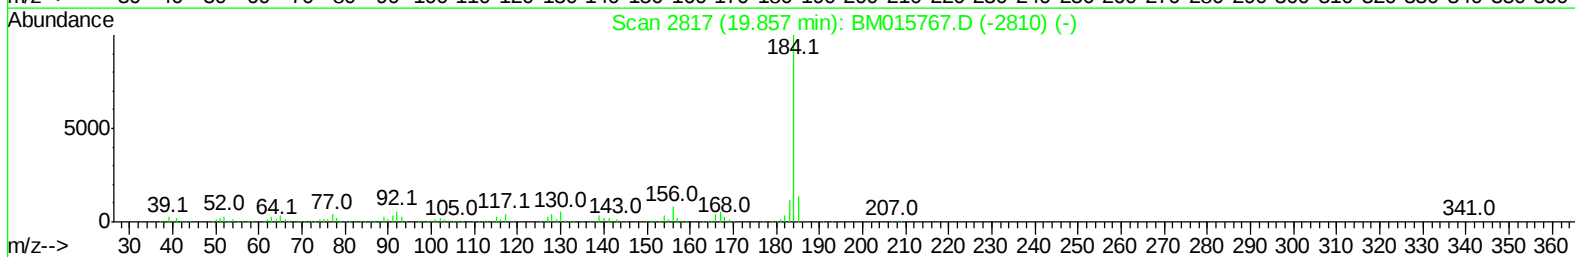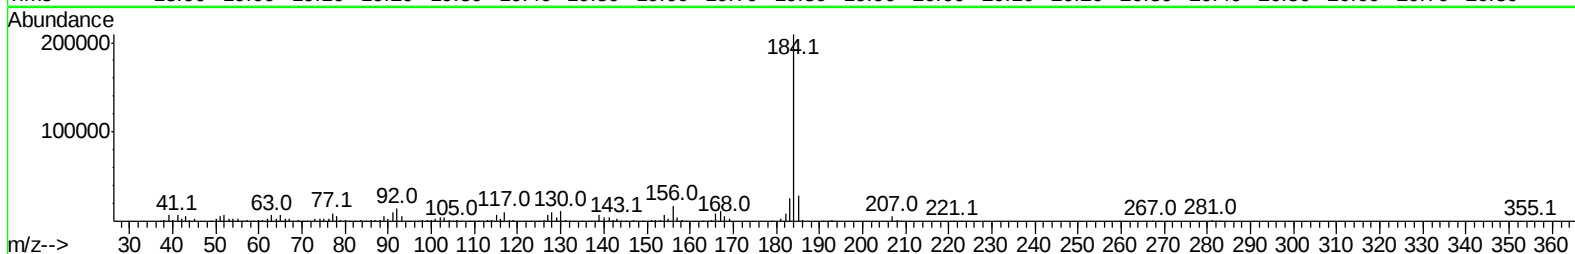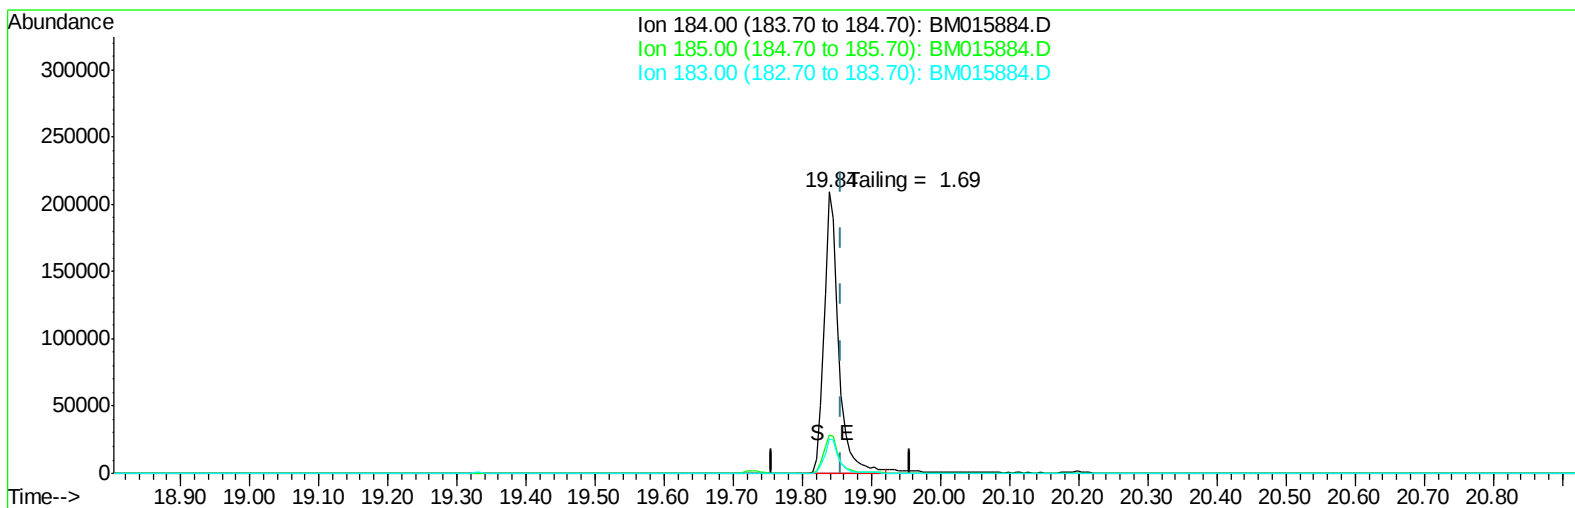

TIC: BM015884.D

(76) Benzidine

19.839min (-0.018) 1952.57ng

response 304977

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.58
183.00	11.10	12.35
0.00	0.00	0.00