
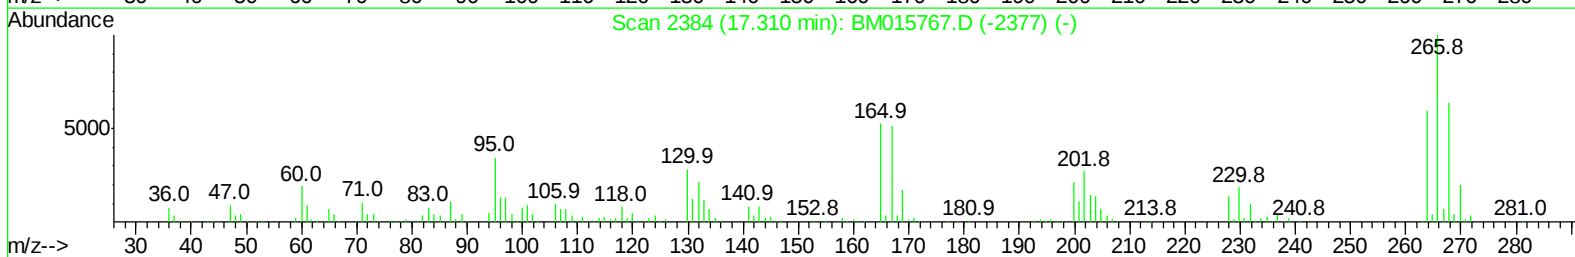
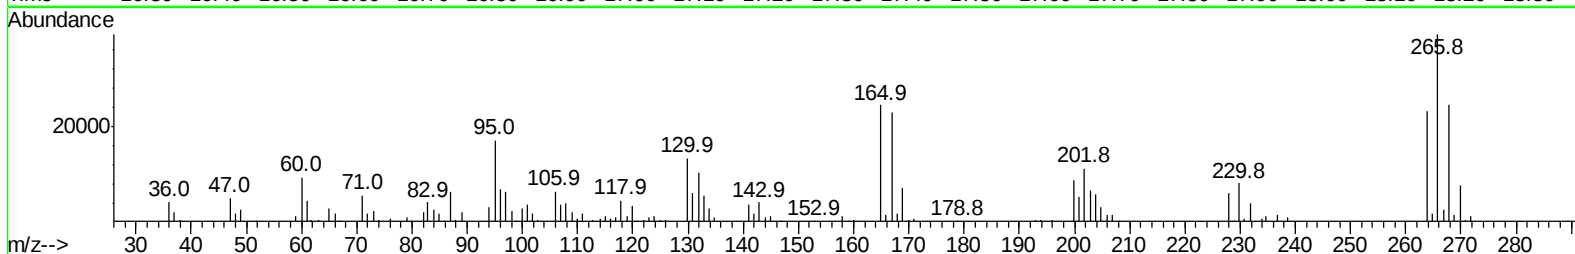


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071118\
Data File : BM015897.D
Acq On : 12 Jul 2018 03:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 09:23:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

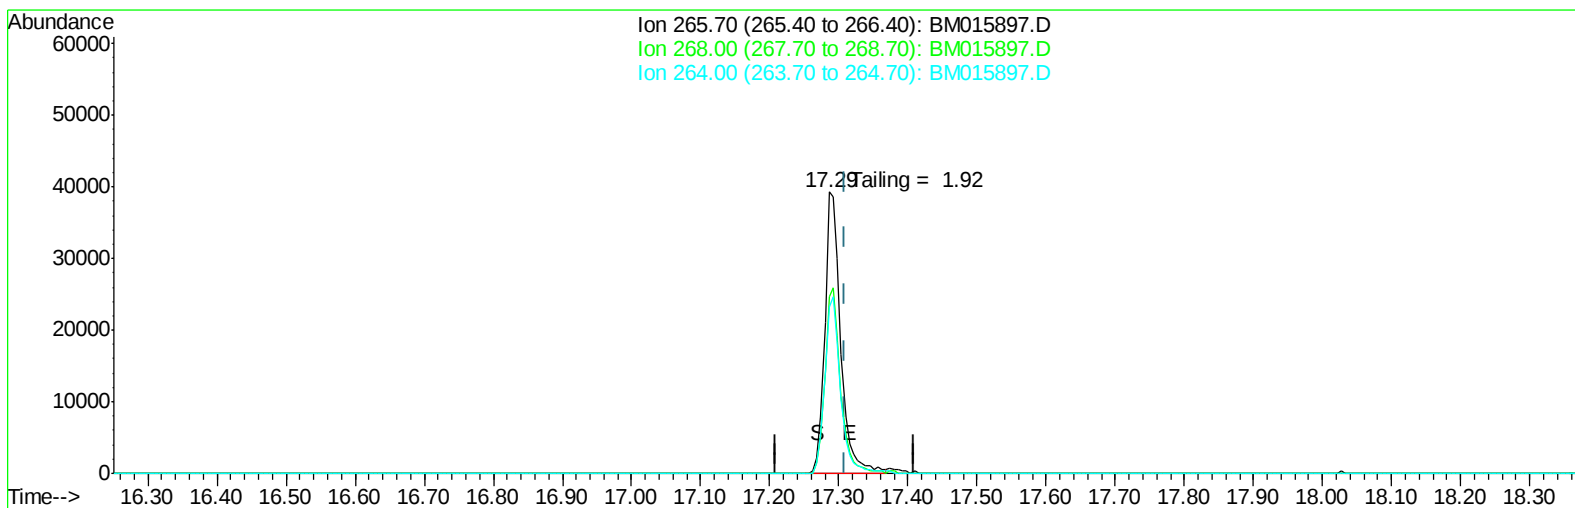

TIC: BM015897.D

(69) Pentachlorophenol (C)




17.286min (-0.024) 0.00ng

response 62947

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.58
264.00	61.20	59.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071118\
 Data File : BM015897.D
 Acq On : 12 Jul 2018 03:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 09:23:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 05 17:39:50 2018
 Response via : Initial Calibration

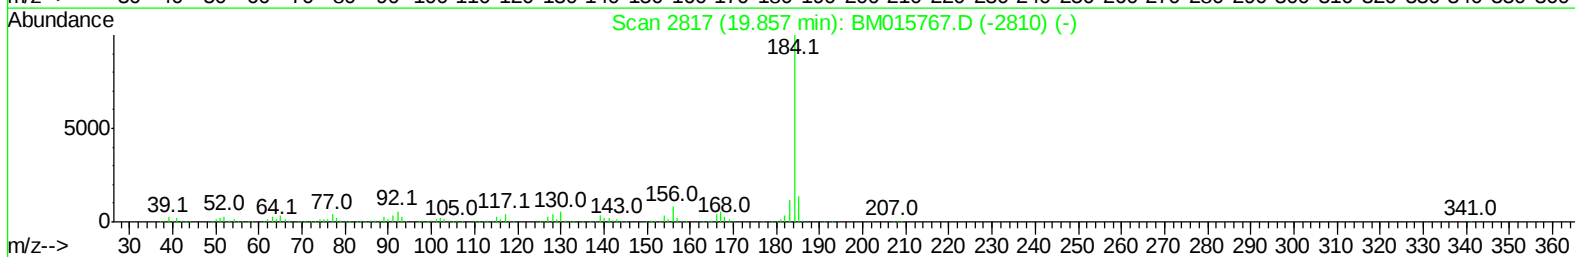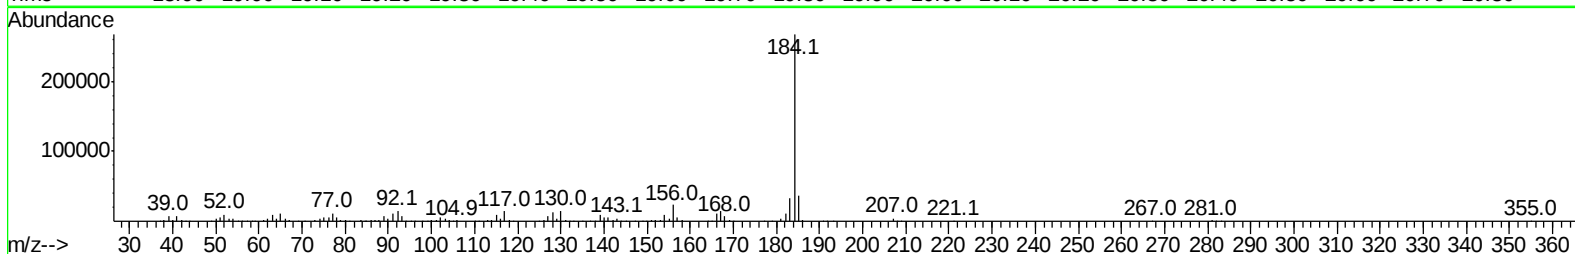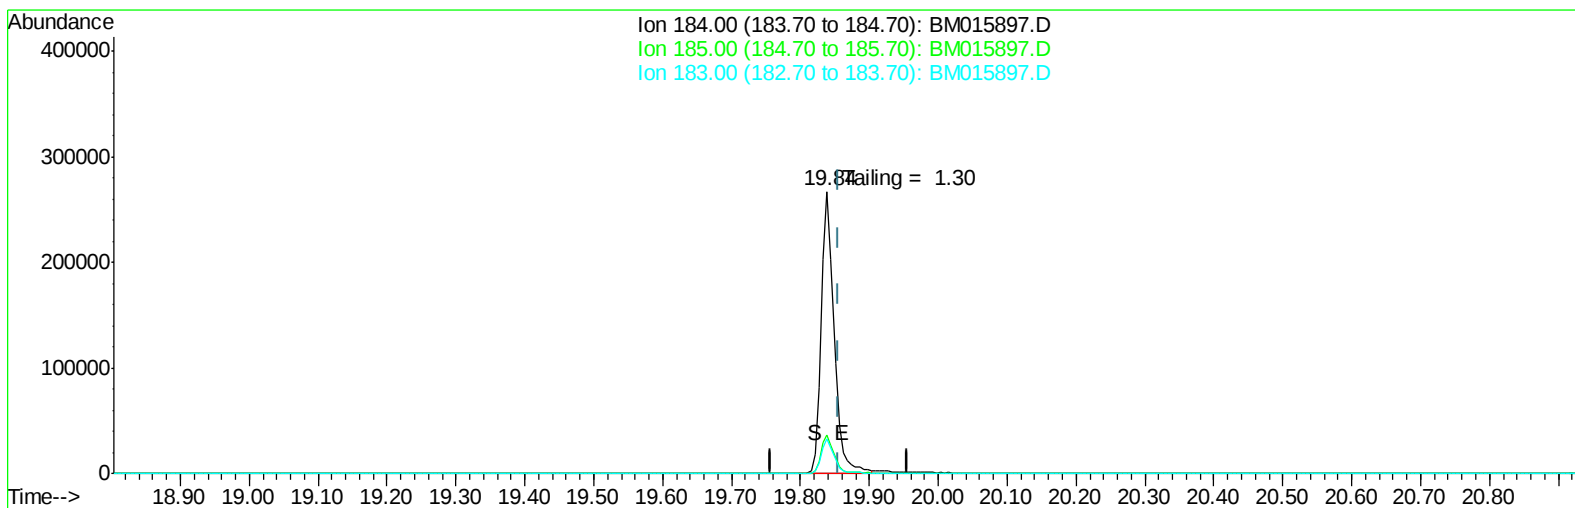

TIC: BM015897.D

(76) Benzidine

19.839min (-0.018) 13437.68ng

response 351189

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.83
183.00	11.10	12.34
0.00	0.00	0.00