

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071118\
 Data File : BM015899.D
 Acq On : 12 Jul 2018 05:25
 Operator : SJ/JU
 Sample : PB111002BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB111002BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.310	339	344	356	rBV	217838	335648	7.56%	1.142%
2	5.793	420	426	442	rBV	1956920	2887182	65.02%	9.824%
3	7.440	700	706	719	rBV	1874698	3043931	68.55%	10.358%
4	7.816	763	770	789	rBV	1950925	3253133	73.26%	11.070%
5	8.287	844	850	863	rBV	338555	572584	12.89%	1.948%
6	8.610	898	905	921	rVB	1439819	2406159	54.19%	8.188%
7	9.475	1045	1052	1071	rBV	1100520	1859708	41.88%	6.328%
8	11.116	1324	1331	1343	rBV	415494	697999	15.72%	2.375%
9	13.539	1736	1743	1763	rBV	2615668	3804515	85.68%	12.946%
10	14.910	1969	1976	1988	rBV2	538783	816198	18.38%	2.777%
11	16.392	2222	2228	2241	rBV	2023100	2824789	63.61%	9.612%
12	17.639	2434	2440	2451	rBV	593611	861776	19.41%	2.932%
13	20.198	2870	2875	2884	rBV	3717419	4440595	100.00%	15.110%
14	21.503	3094	3097	3101	rBV	41077	53333	1.20%	0.181%
15	21.750	3134	3139	3147	rBV	587013	802526	18.07%	2.731%
16	24.144	3540	3546	3555	rVB	356941	727968	16.39%	2.477%


Sum of corrected areas: 29388044

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071118\
Data File : BM015899.D
Acq On : 12 Jul 2018 05:25
Operator : SJ/JU
Sample : PB111002BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB111002BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

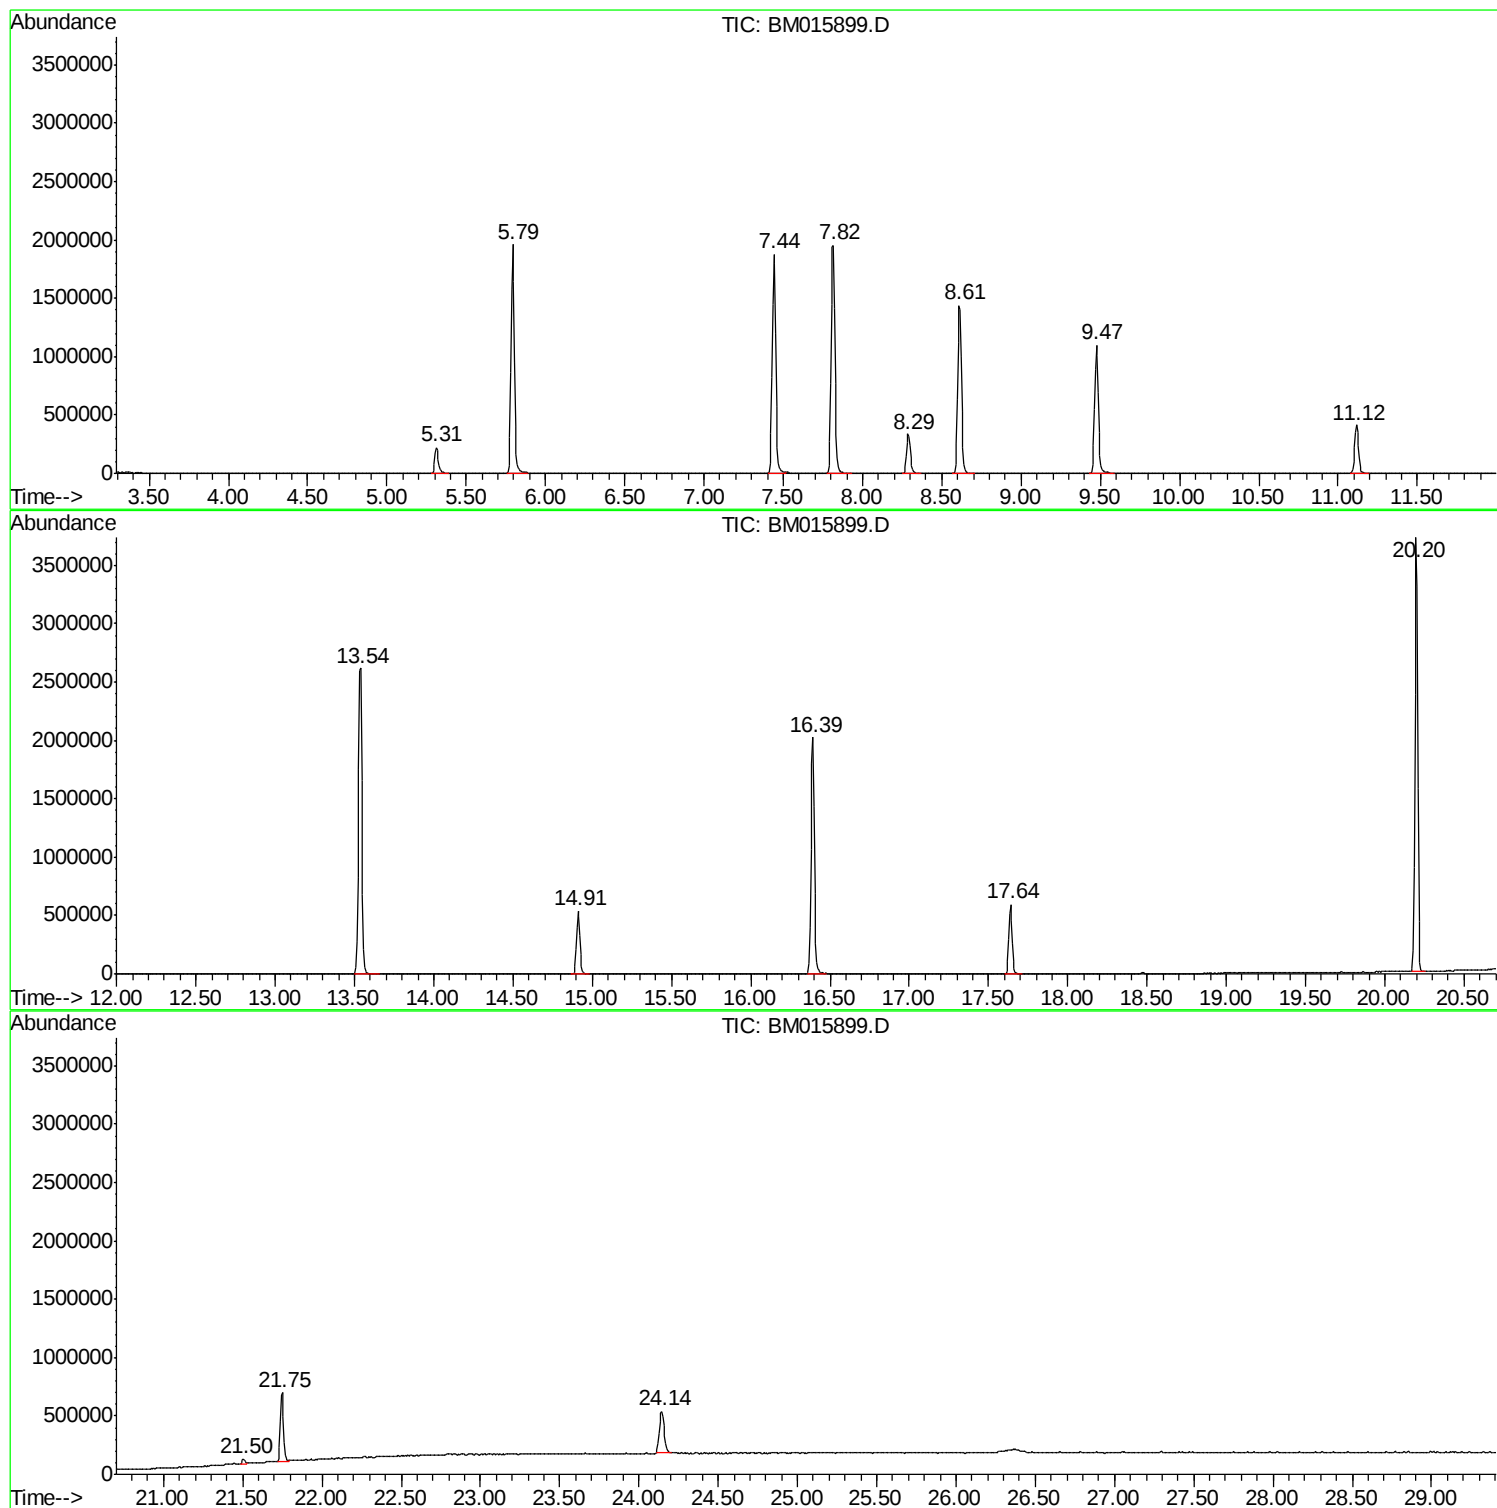

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071118\
Data File : BM015899.D
Acq On : 12 Jul 2018 05:25
Operator : SJ/JU
Sample : PB111002BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB111002BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.31	11.72 ng	335648	1,4-Dichlorobenzene-d4	8.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		1-Butene, 4-ethoxy-	100	C6H12O	044611-46-3	23
3		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
4		Butane	58	C4H10	000106-97-8	9
5		Propylamine	59	C3H9N	000107-10-8	9

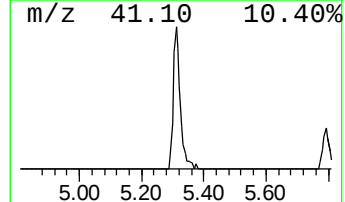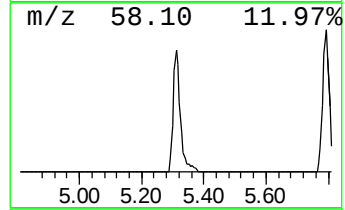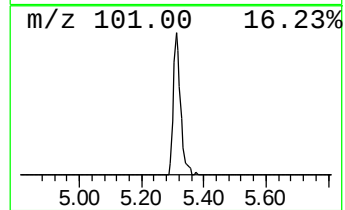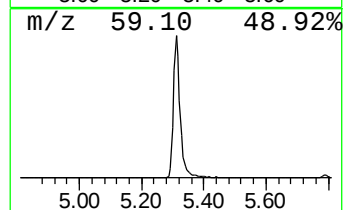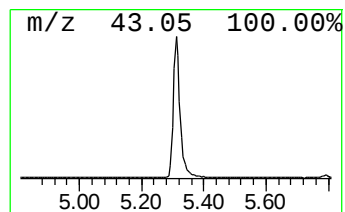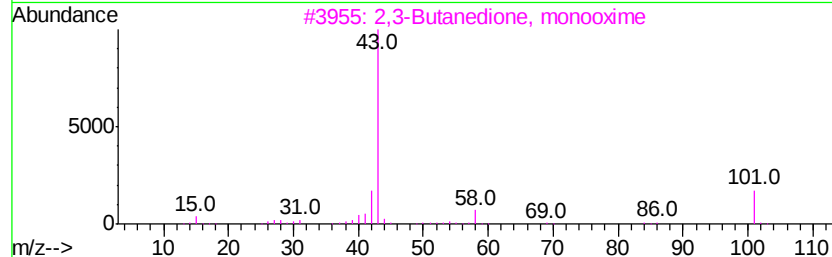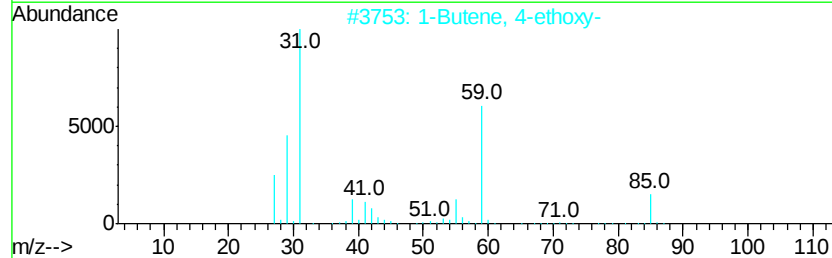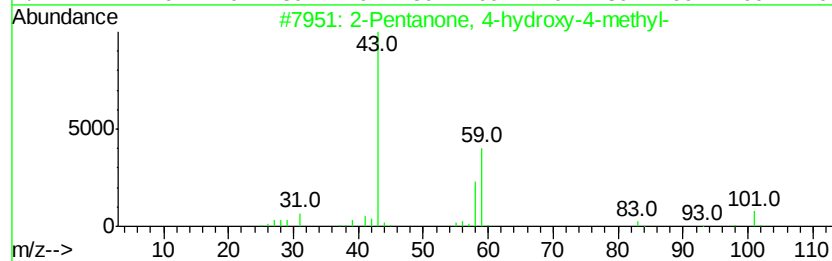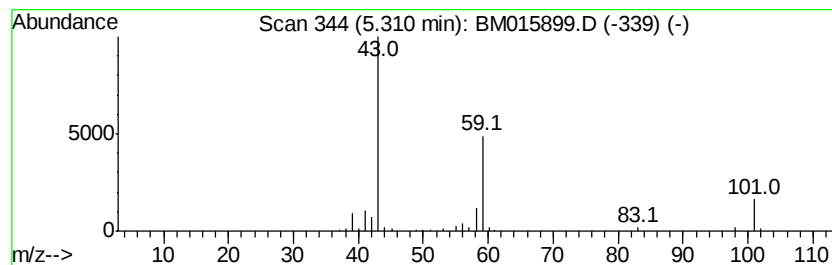

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071118\
Data File : BM015899.D
Acq On : 12 Jul 2018 05:25
Operator : SJ/JU
Sample : PB111002BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB111002BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.82 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.82	113.63 ng	3253130	1,4-Dichlorobenzene-d4	8.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	27
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	22
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClfFN2	1000146-10-7	16
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	14

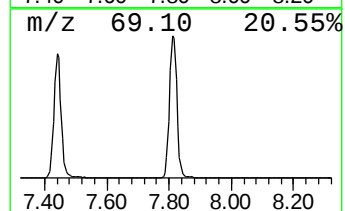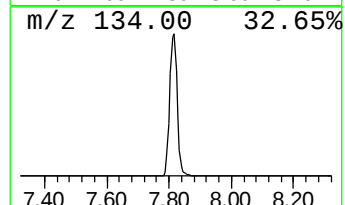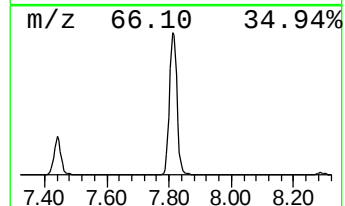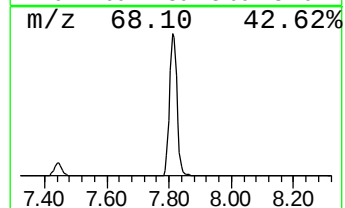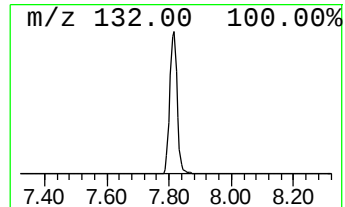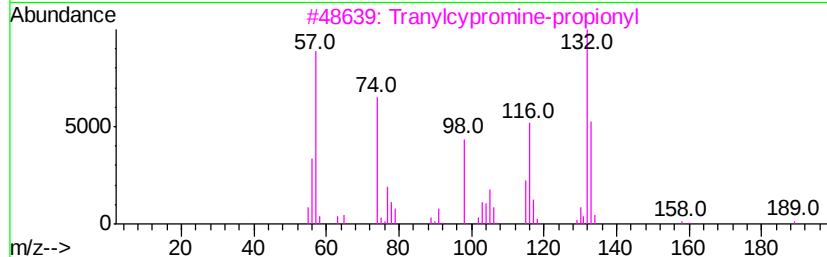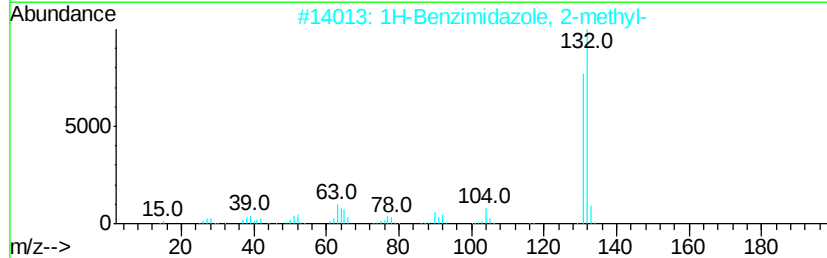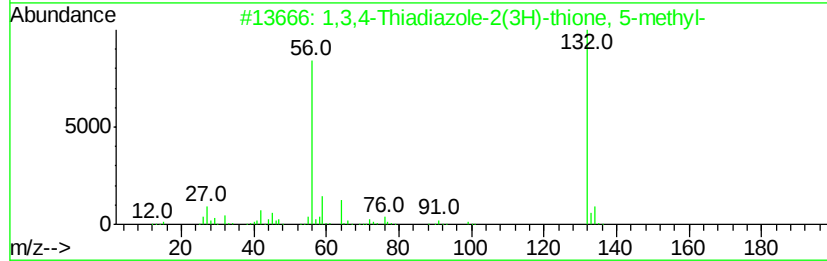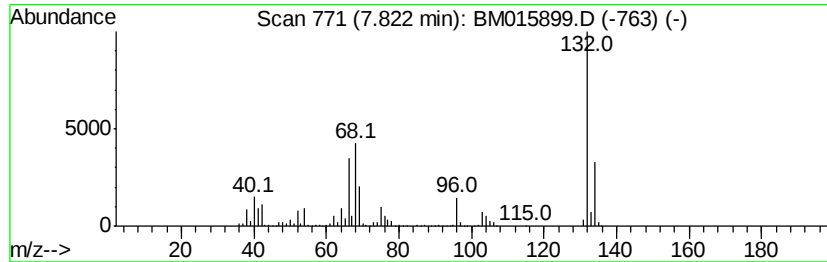

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071118\
Data File : BM015899.D
Acq On : 12 Jul 2018 05:25
Operator : SJ/JU
Sample : PB111002BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB111002BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.31	11.7	ng	335648	1	8.29	572584	20.0
unknown7.82	7.82	113.6	ng	3253130	1	8.29	572584	20.0