


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071118\
 Data File : BM015897.D
 Acq On : 12 Jul 2018 03:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

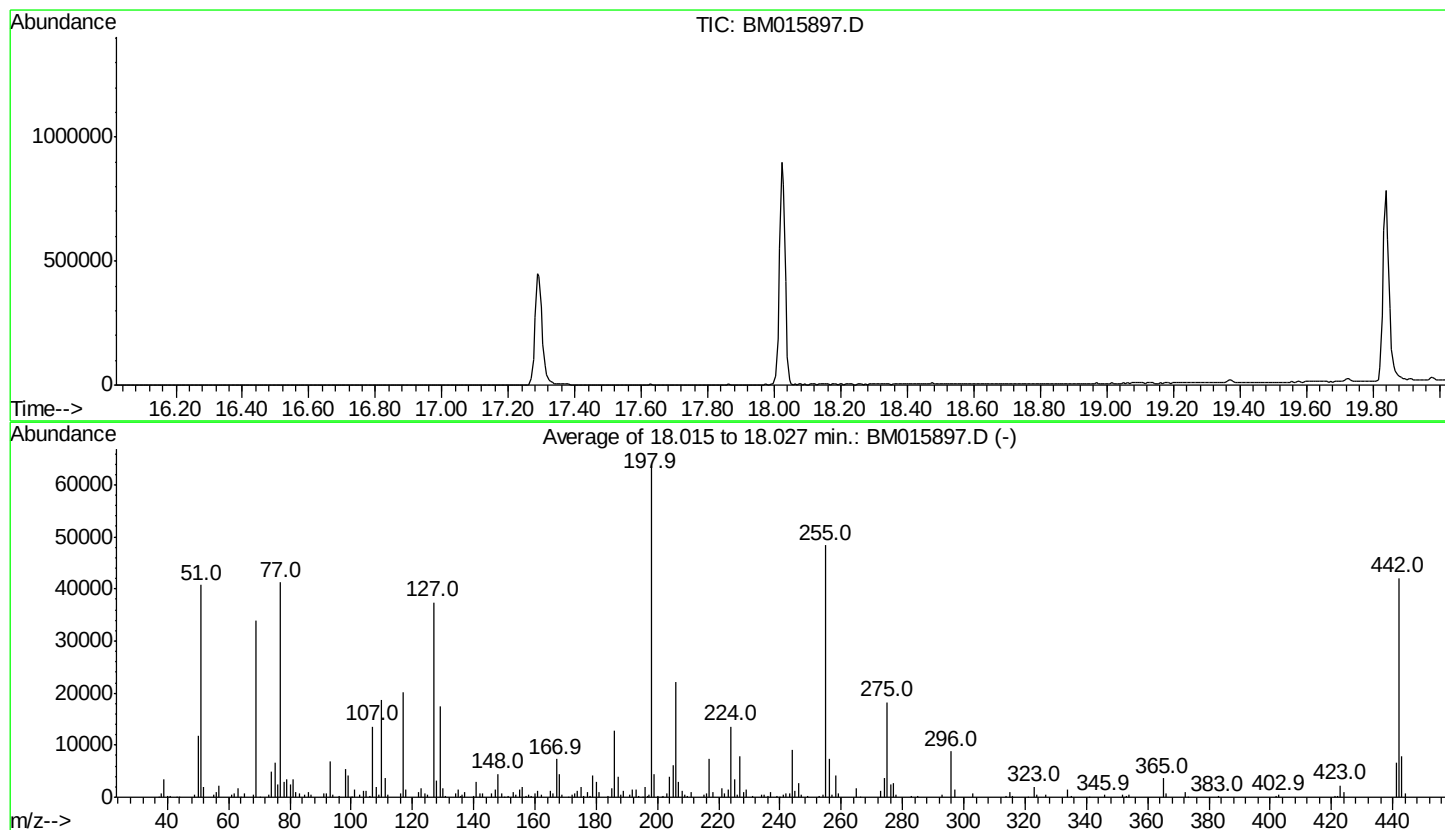

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.0	40773	PASS
68	69	0.00	2	1.8	621	PASS
69	198	0.00	100	53.2	33901	PASS
70	69	0.00	2	0.4	131	PASS
127	198	10	80	58.8	37474	PASS
197	198	0.00	2	0.6	390	PASS
198	198	100	100	100.0	63682	PASS
199	198	5	9	6.9	4396	PASS
275	198	10	60	28.7	18287	PASS
365	198	1	100	5.6	3576	PASS
441	443	0.01	100	84.3	6656	PASS
442	198	50	100	66.2	42146	PASS
443	442	15	24	18.7	7899	PASS