

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071119\
 Data File : BM021430.D
 Acq On : 11 Jul 2019 16:30
 Operator : HP/JU
 Sample : PB121271BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.910	661	667	679	rVB	632801	1027947	25.09%	2.719%
2	7.075	690	695	704	rVB	475992	769776	18.79%	2.036%
3	7.269	721	728	737	rVB	686842	1121356	27.37%	2.966%
4	7.734	801	807	814	rVB	488339	781886	19.08%	2.068%
5	8.440	921	927	941	rVB	776525	1272348	31.05%	3.366%
6	8.892	998	1004	1012	rBV	620792	1033052	25.21%	2.733%
7	9.610	1119	1126	1139	rBV	518180	842257	20.56%	2.228%
8	10.145	1210	1217	1240	rVB	767845	1383079	33.75%	3.659%
9	10.516	1273	1280	1288	rBV	620394	1055757	25.77%	2.793%
10	10.669	1299	1306	1330	rVB	671086	1305102	31.85%	3.452%
11	12.122	1550	1553	1560	rVB4	8884	15280	0.37%	0.040%
12	13.792	1831	1837	1847	rBV	1428825	1999918	48.81%	5.290%
13	14.069	1877	1884	1899	rBV	1722823	2466745	60.20%	6.525%
14	14.374	1929	1936	1947	rBV2	922928	1410438	34.42%	3.731%
15	14.598	1968	1974	1991	rBV	368522	691814	16.88%	1.830%
16	15.374	2099	2106	2116	rBV	2122316	3097575	75.60%	8.194%
17	15.510	2123	2129	2143	rBV	404422	623127	15.21%	1.648%
18	15.616	2143	2147	2153	rVB	22708	31601	0.77%	0.084%
19	16.157	2235	2239	2244	rBV3	6226	8910	0.22%	0.024%
20	16.921	2365	2369	2372	rBV2	3944	6031	0.15%	0.016%
21	17.127	2398	2404	2413	rBV2	1230916	1673962	40.85%	4.428%
22	17.227	2414	2421	2434	rBV	2277920	3284004	80.15%	8.687%
23	19.157	2746	2749	2754	rVB	17692	23999	0.59%	0.063%
24	19.415	2789	2793	2796	rBV2	16752	21769	0.53%	0.058%
25	19.527	2805	2812	2822	rBV	2742438	3867233	94.38%	10.230%
26	21.315	3111	3116	3125	rBV	1438605	1967044	48.01%	5.204%
27	23.433	3469	3476	3490	rVB	2228333	4097533	100.00%	10.839%
28	23.574	3495	3500	3509	rVB	1003293	1922549	46.92%	5.086%


Sum of corrected areas: 37802092

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071119\
Data File : BM021430.D
Acq On : 11 Jul 2019 16:30
Operator : HP/JU
Sample : PB121271BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

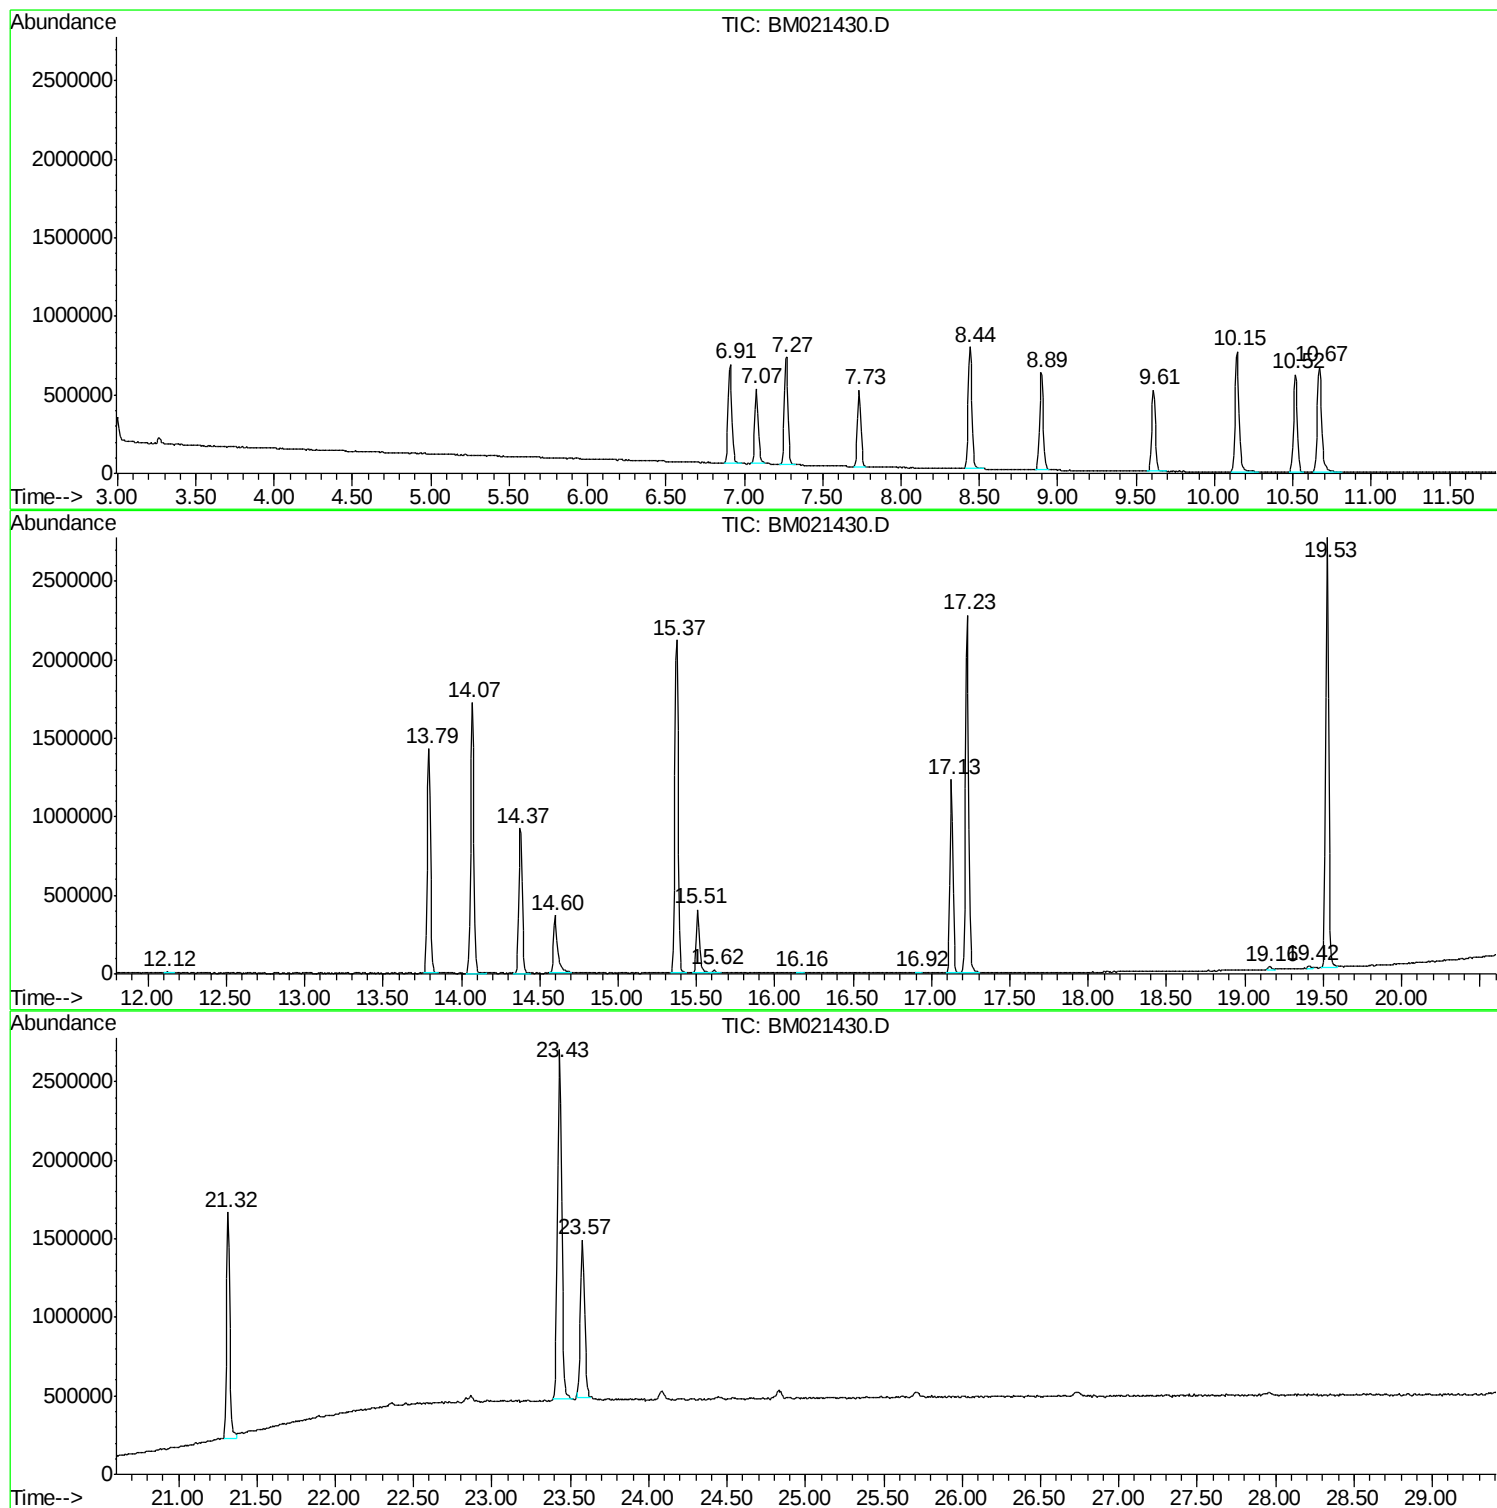

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071119\
Data File : BM021430.D
Acq On : 11 Jul 2019 16:30
Operator : HP/JU
Sample : PB121271BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071119\
Data File : BM021430.D
Acq On : 11 Jul 2019 16:30
Operator : HP/JU
Sample : PB121271BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc