

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071119\
 Data File : BM021446.D
 Acq On : 12 Jul 2019 02:16
 Operator : HP/JU
 Sample : PB121315BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.904	660	666	680	rVB	728401	1185954	23.70%	2.471%
2	7.075	689	695	706	rVB	578244	909365	18.17%	1.895%
3	7.263	721	727	738	rVB	823623	1305397	26.09%	2.720%
4	7.728	800	806	814	rVB	693867	1119569	22.37%	2.333%
5	8.439	920	927	942	rVB	908943	1507516	30.13%	3.141%
6	8.892	997	1004	1017	rVB	744258	1234636	24.67%	2.573%
7	9.610	1119	1126	1136	rVB	616124	1022893	20.44%	2.131%
8	10.139	1209	1216	1235	rBV	953476	1650154	32.98%	3.438%
9	10.516	1272	1280	1287	rBV	964376	1571711	31.41%	3.275%
10	10.663	1298	1305	1325	rBV	812369	1584260	31.66%	3.301%
11	12.122	1549	1553	1560	rVB	11809	19971	0.40%	0.042%
12	13.792	1830	1837	1848	rBV	1731008	2423566	48.43%	5.050%
13	14.068	1876	1884	1894	rBV	2039635	2964263	59.24%	6.177%
14	14.374	1929	1936	1948	rBV2	1412823	2132328	42.61%	4.443%
15	14.598	1967	1974	1994	rBV	461362	895938	17.91%	1.867%
16	15.374	2099	2106	2119	rBV	2472919	3716399	74.27%	7.744%
17	15.504	2123	2128	2142	rBV	510514	785545	15.70%	1.637%
18	15.615	2142	2147	2151	rVB	26680	34341	0.69%	0.072%
19	16.157	2235	2239	2242	rVB4	8912	11261	0.23%	0.023%
20	16.909	2364	2367	2373	rVB3	6279	10124	0.20%	0.021%
21	17.127	2397	2404	2414	rBV	1901186	2548918	50.94%	5.311%
22	17.227	2414	2421	2433	rBV	2709473	3927025	78.48%	8.183%
23	18.886	2701	2703	2707	rBV4	4513	5982	0.12%	0.012%
24	19.156	2745	2749	2755	rBV	24053	34060	0.68%	0.071%
25	19.409	2789	2792	2795	rBV	20516	24069	0.48%	0.050%
26	19.521	2805	2811	2823	rBV	3386245	4582437	91.58%	9.548%
27	21.315	3111	3116	3124	rBV	2148489	2828002	56.52%	5.893%
28	23.427	3469	3475	3486	rVB	2787877	5003814	100.00%	10.427%
29	23.574	3494	3500	3511	rVB	1518776	2951791	58.99%	6.151%


Sum of corrected areas: 47991289

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071119\
Data File : BM021446.D
Acq On : 12 Jul 2019 02:16
Operator : HP/JU
Sample : PB121315BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

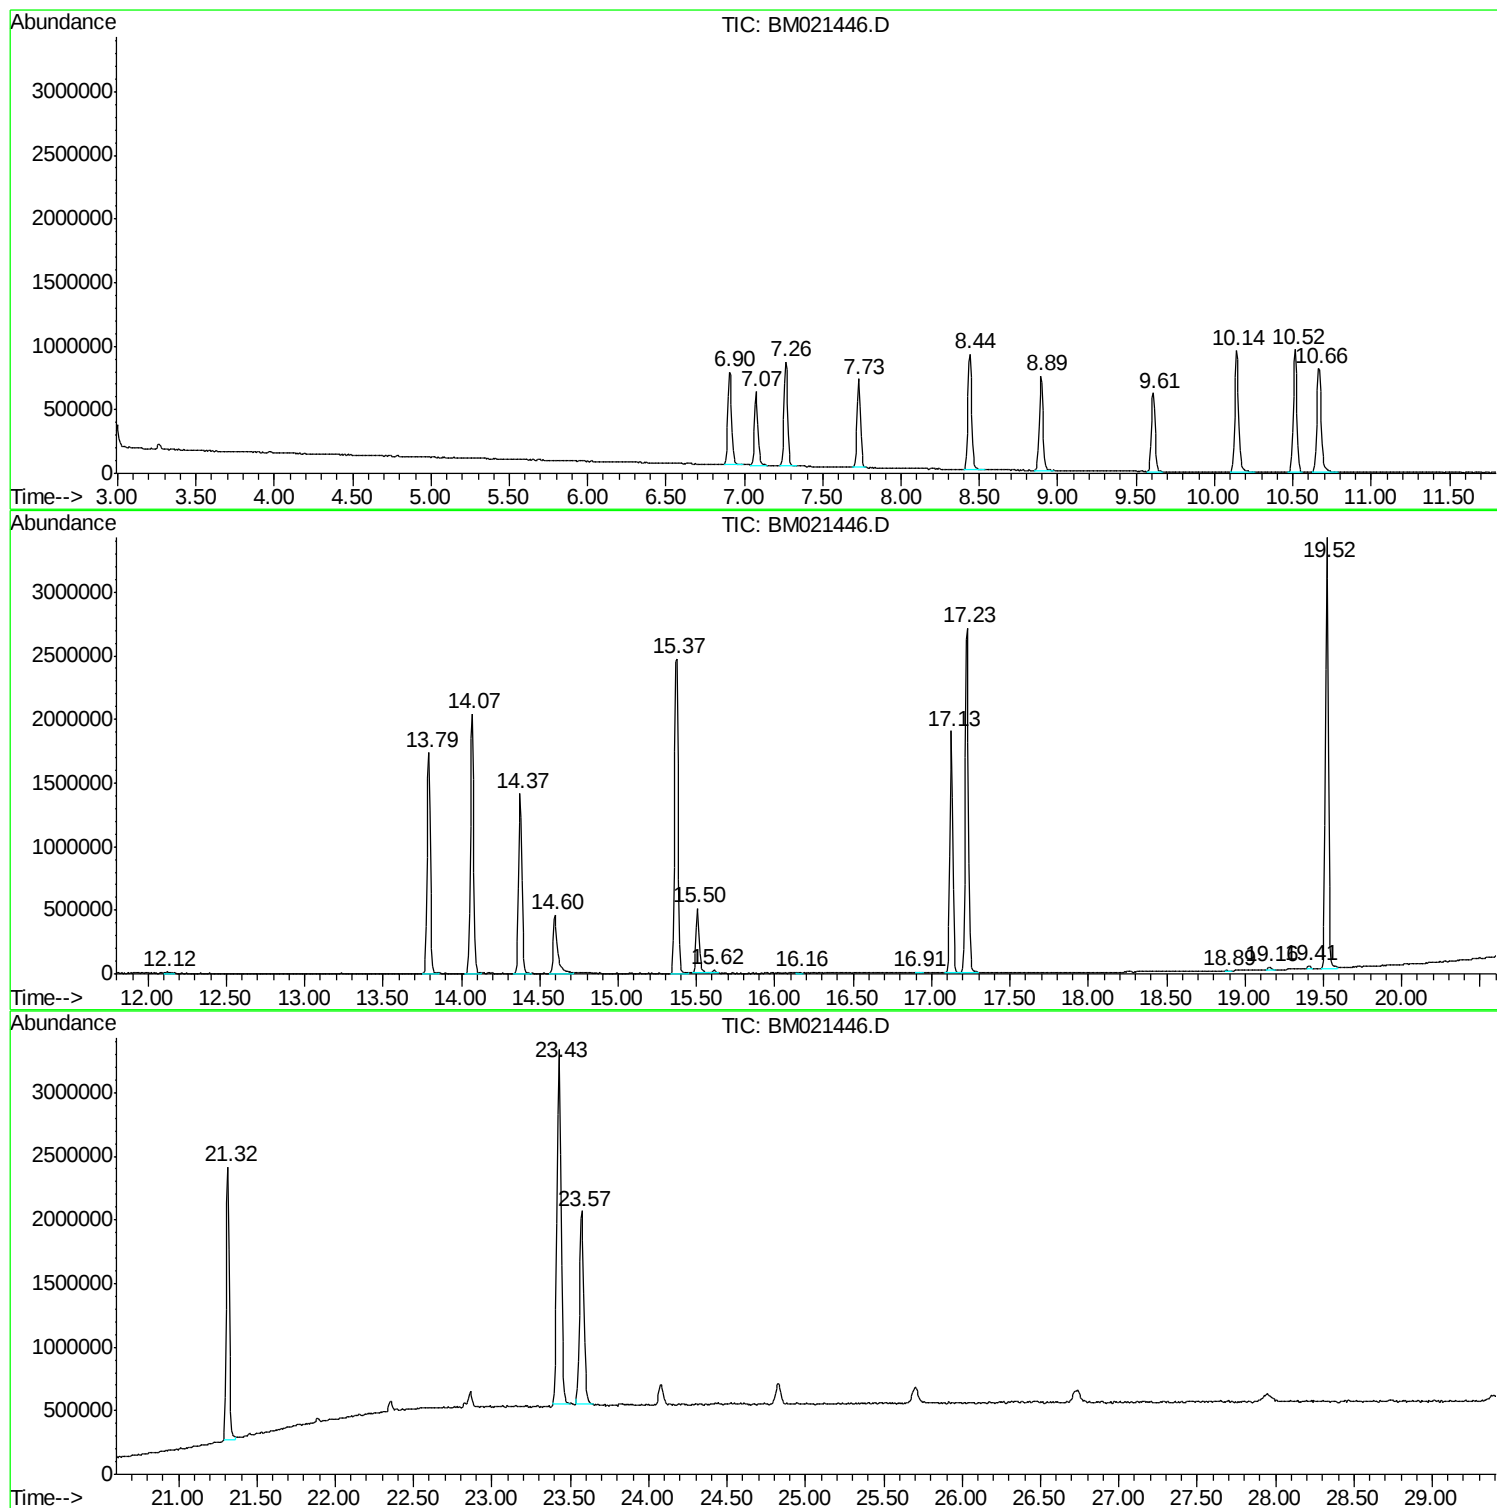

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071119\
Data File : BM021446.D
Acq On : 12 Jul 2019 02:16
Operator : HP/JU
Sample : PB121315BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071119\
Data File : BM021446.D
Acq On : 12 Jul 2019 02:16
Operator : HP/JU
Sample : PB121315BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc