

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040810.D
 Acq On : 11 Jul 2023 13:25
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Quant Time: Jul 12 04:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.883	152	3942	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	13829	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	6845	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	12209	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	6965	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.88
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	33112	5.347	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	5644	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.311	212	6791	0.304	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.522	166	2199	0.080	ng/ul#	17
20) Pyrene	19.673	202	1365	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040810.D
Acq On : 11 Jul 2023 13:25
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK963

Quant Time: Jul 12 04:33:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration




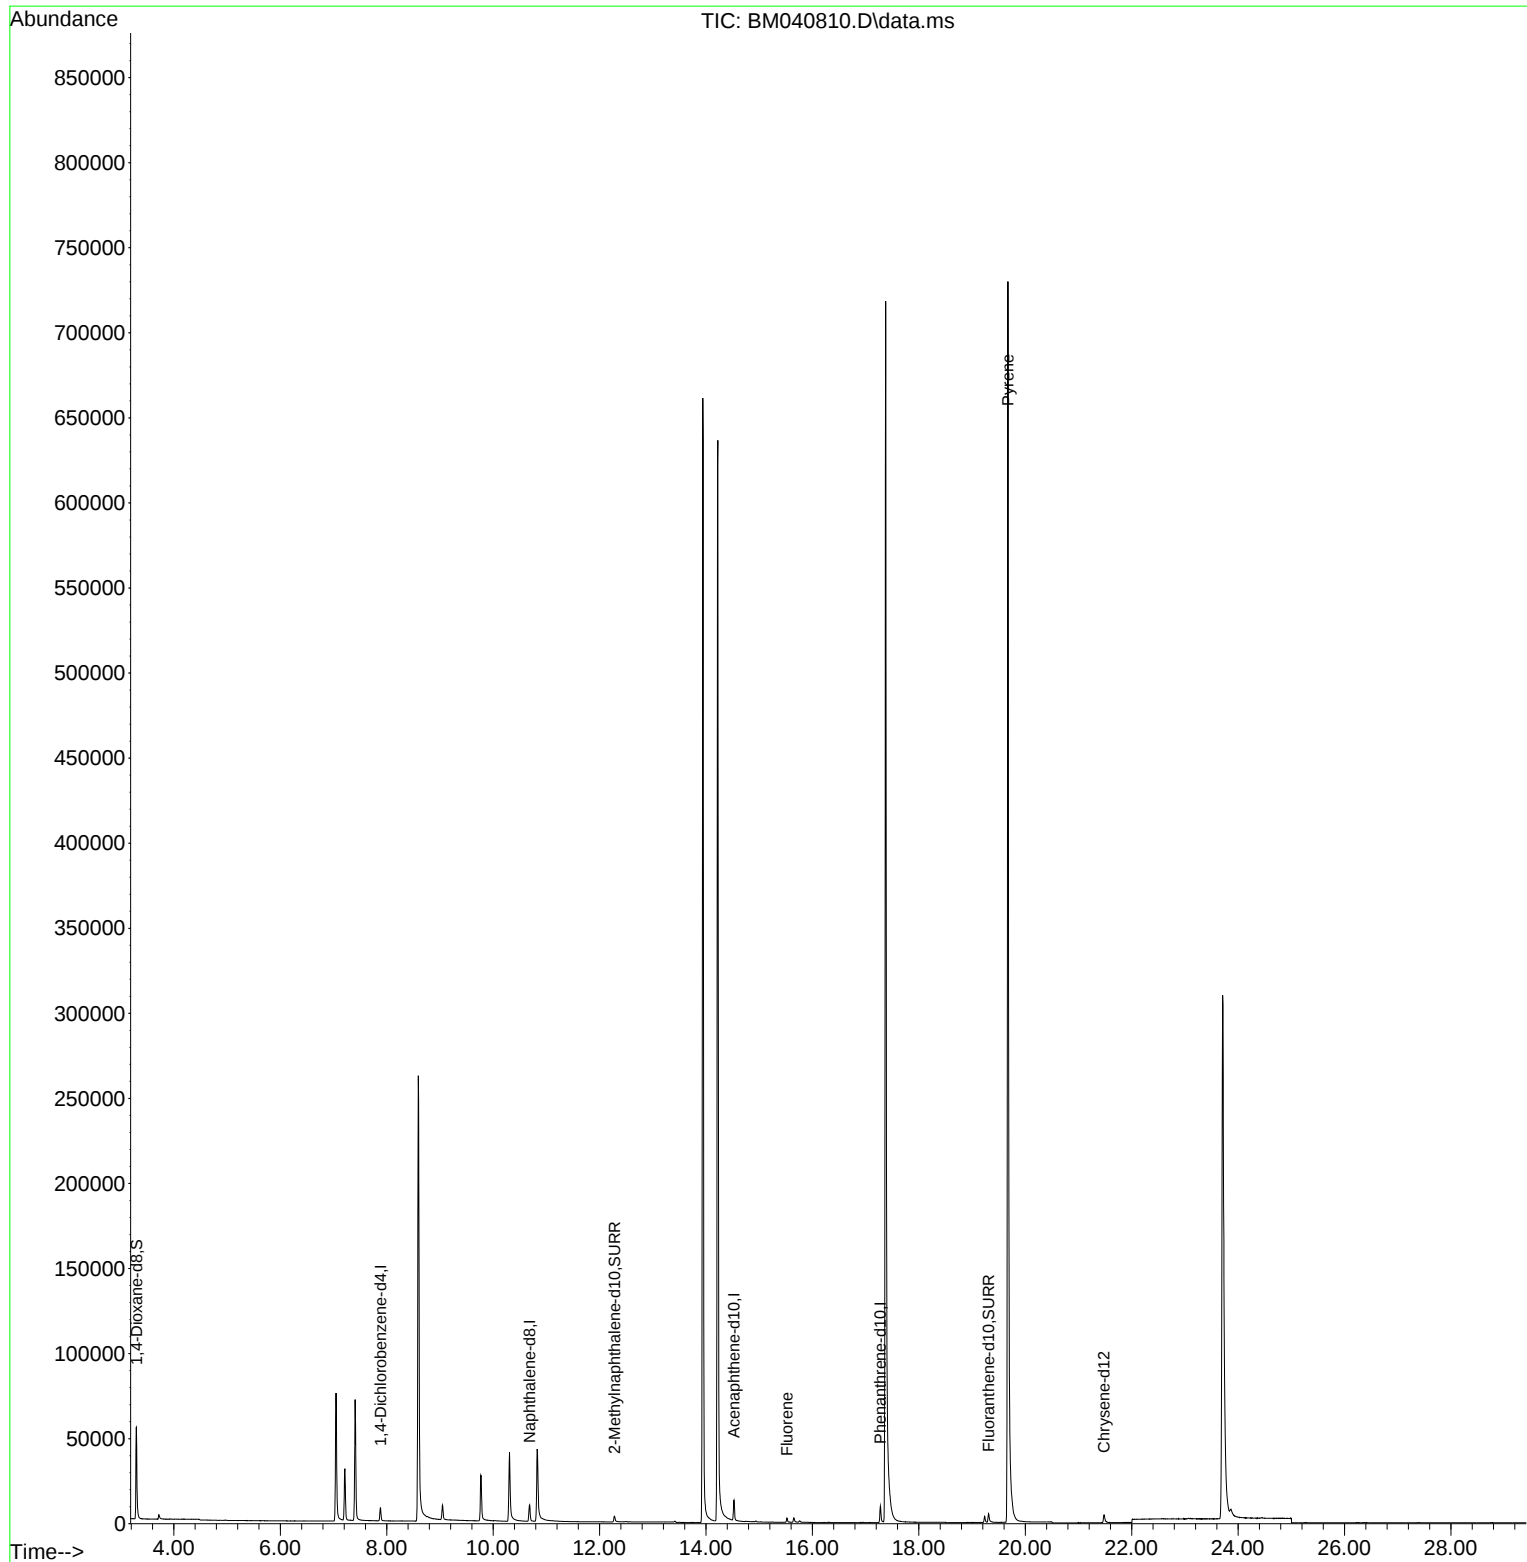


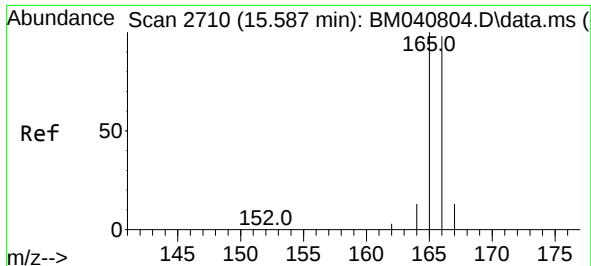

#12
Fluorene
Concen: 0.080 ng/ul
RT: 15.522 min Scan# 2199
Delta R.T. -0.069 min
Lab File: BM040810.D
Acq: 11 Jul 2023 13:25

Instrument :
BNA_M
ClientSampleId :
SBLK963

Tgt Ion:166 Resp: 2199
Ion Ratio Lower Upper
166 100
165 11.2 79.6 119.4#
167 33.5 11.4 17.0#

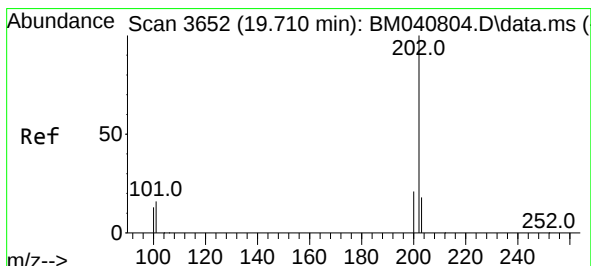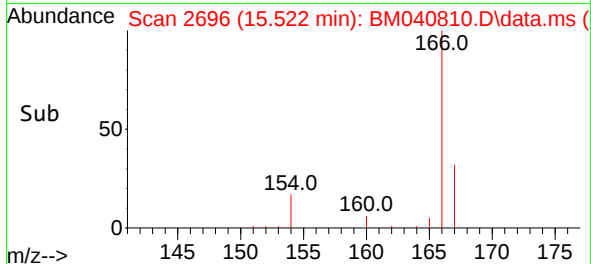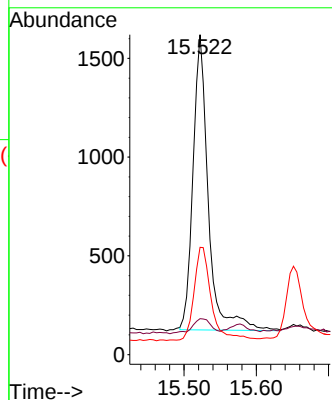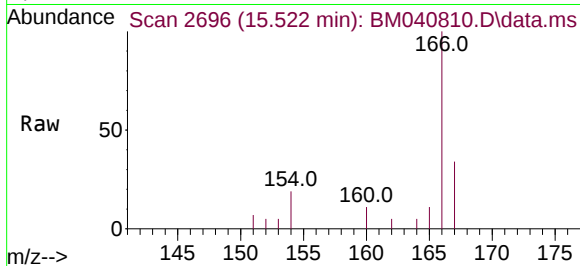

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.673 min Scan# 3644
Delta R.T. -0.042 min
Lab File: BM040810.D
Acq: 11 Jul 2023 13:25

Tgt Ion:202 Resp: 1365
Ion Ratio Lower Upper
202 100
101 203.3 12.6 18.8#
100 1533.4 9.8 14.6#

