

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040815.D
 Acq On : 11 Jul 2023 16:45
 Operator : MA/JU
 Sample : PB154053BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK053

Quant Time: Jul 12 04:34:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3311	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	12094	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	6020	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	10866	0.400	ng/ul	-0.01
17) Chrysene-d12	21.483	240	6565	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.88
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	34980	6.726	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	6088	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	8247	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.522	166	2443	0.101	ng/ul#	17
20) Pyrene	19.673	202	1755	0.059	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040815.D
Acq On : 11 Jul 2023 16:45
Operator : MA/JU
Sample : PB154053BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Time: Jul 12 04:34:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration




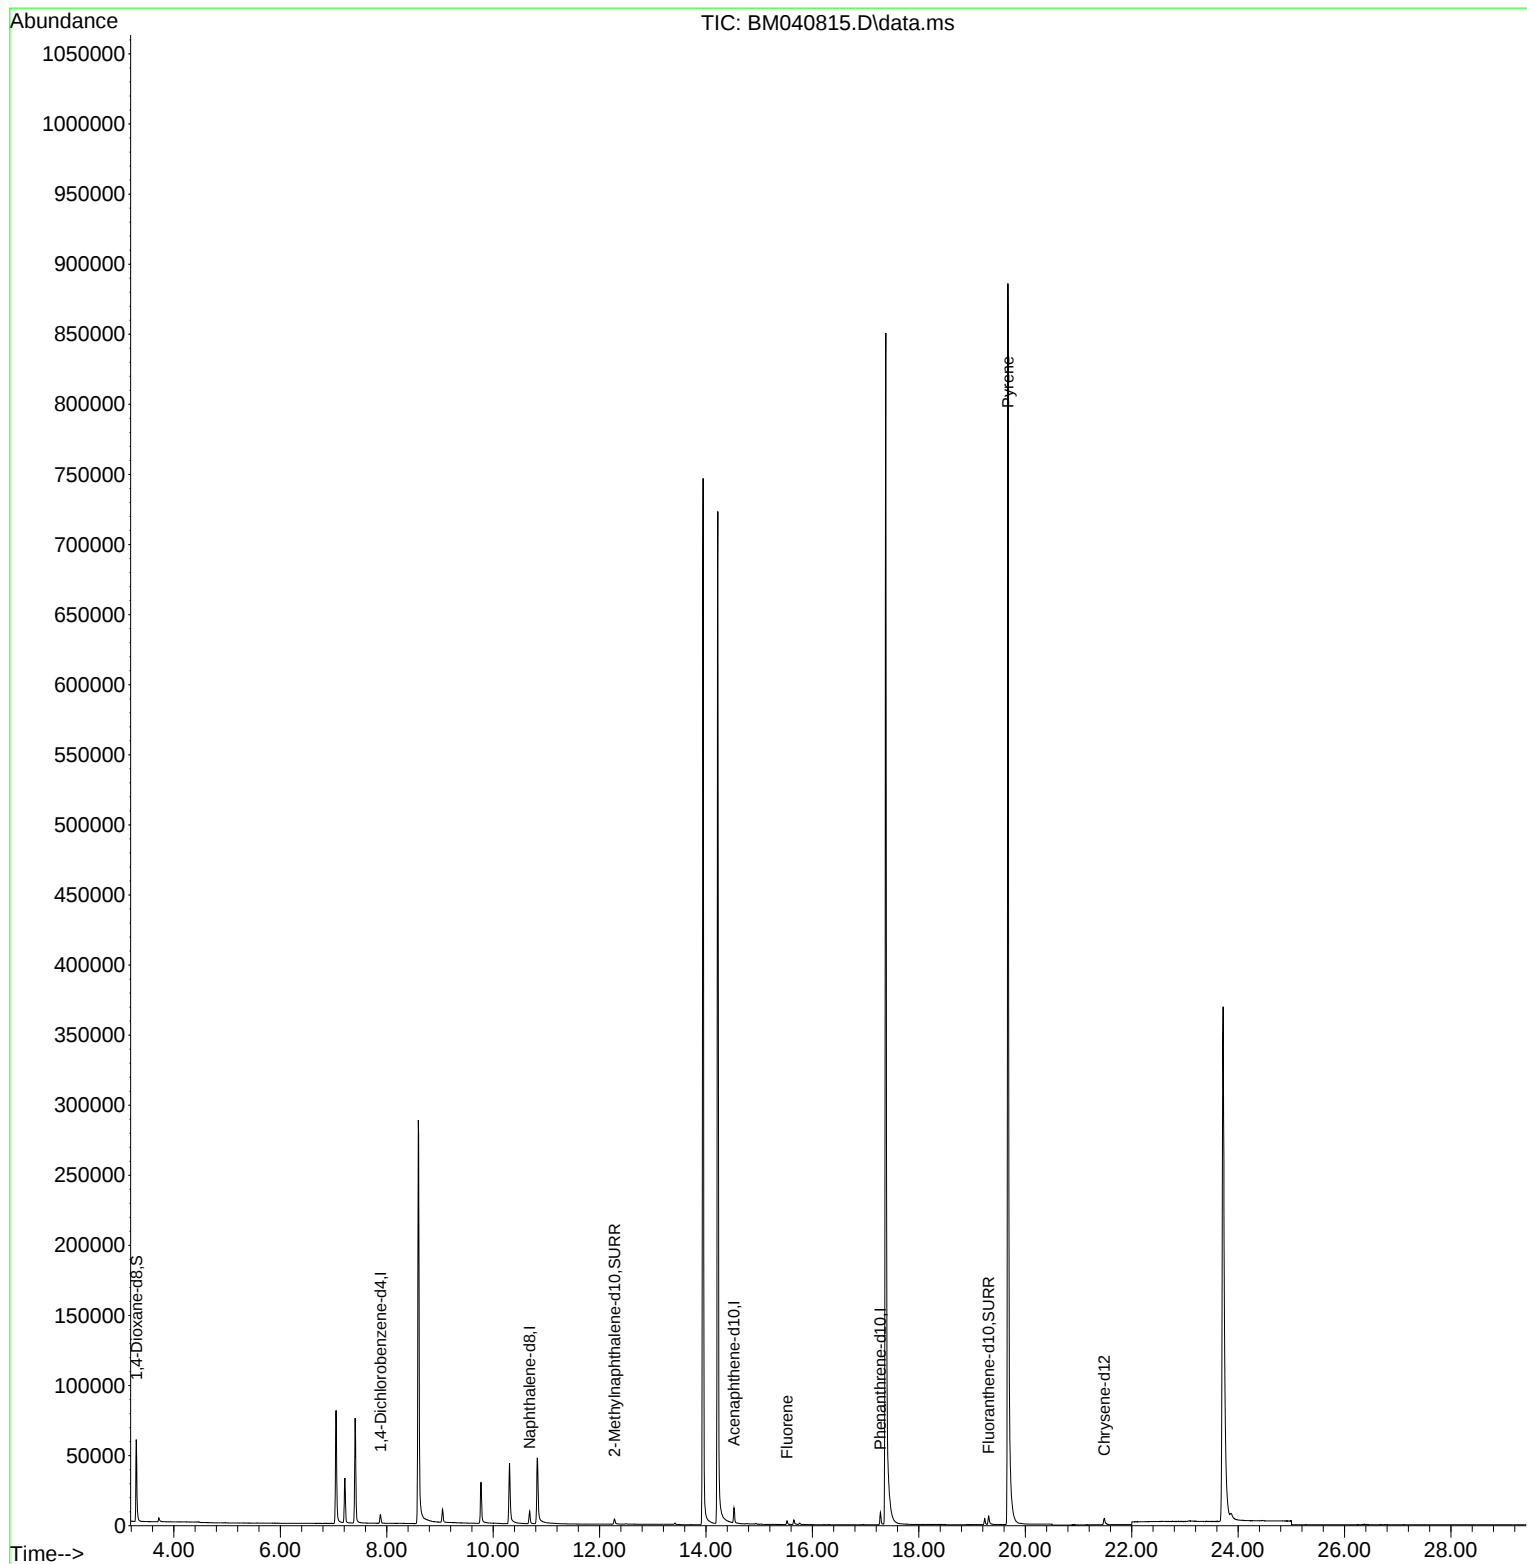


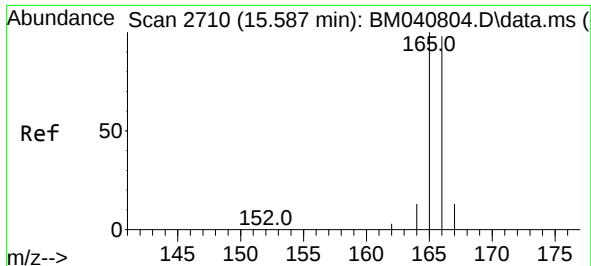

#12
Fluorene
Concen: 0.101 ng/ul
RT: 15.522 min Scan# 21
Delta R.T. -0.069 min
Lab File: BM040815.D
Acq: 11 Jul 2023 16:45

Instrument :
BNA_M
ClientSampleId :
SBLK053

Tgt Ion:166 Resp: 2443
Ion Ratio Lower Upper
166 100
165 11.3 79.6 119.4#
167 33.1 11.4 17.0#

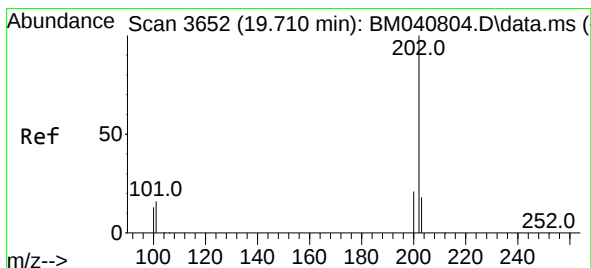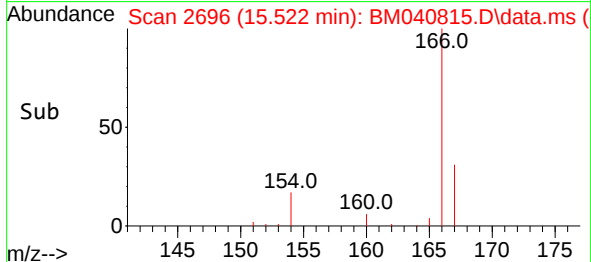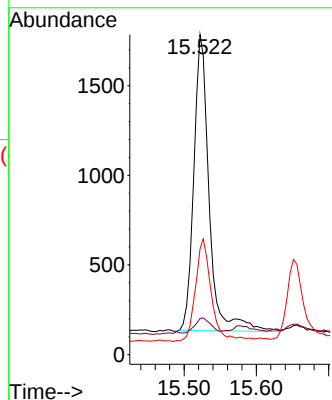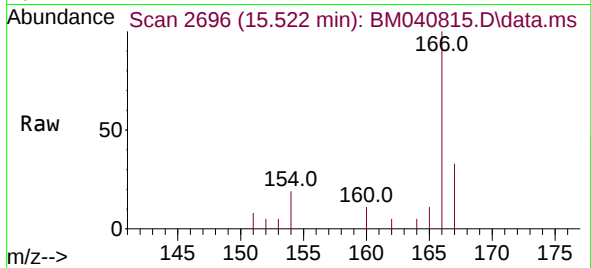

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.673 min Scan# 3644
Delta R.T. -0.042 min
Lab File: BM040815.D
Acq: 11 Jul 2023 16:45

Tgt Ion:202 Resp: 1755
Ion Ratio Lower Upper
202 100
101 194.5 12.6 18.8#
100 1488.5 9.8 14.6#

