

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040818.D
 Acq On : 11 Jul 2023 18:38
 Operator : MA/JU
 Sample : 03414-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD0.4170

Quant Time: Jul 12 04:35:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3505	0.400	ng/ul	0.00
4) Naphthalene-d8	10.685	136	13033	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.532	164	5773	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.286	188	9228	0.400	ng/ul	0.00
17) Chrysene-d12	21.480	240	6833	0.400	ng/ul	0.00
23) Perylene-d12	23.871	264	5812	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.279	96	23	0.004	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.291	152	4	0.000	ng/ul	0.00
18) Fluoranthene-d10	19.324	212	8	0.000	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.740	128	4797	0.133	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040818.D
Acq On : 11 Jul 2023 18:38
Operator : MA/JU
Sample : 03414-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD0.4170


Quant Time: Jul 12 04:35:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

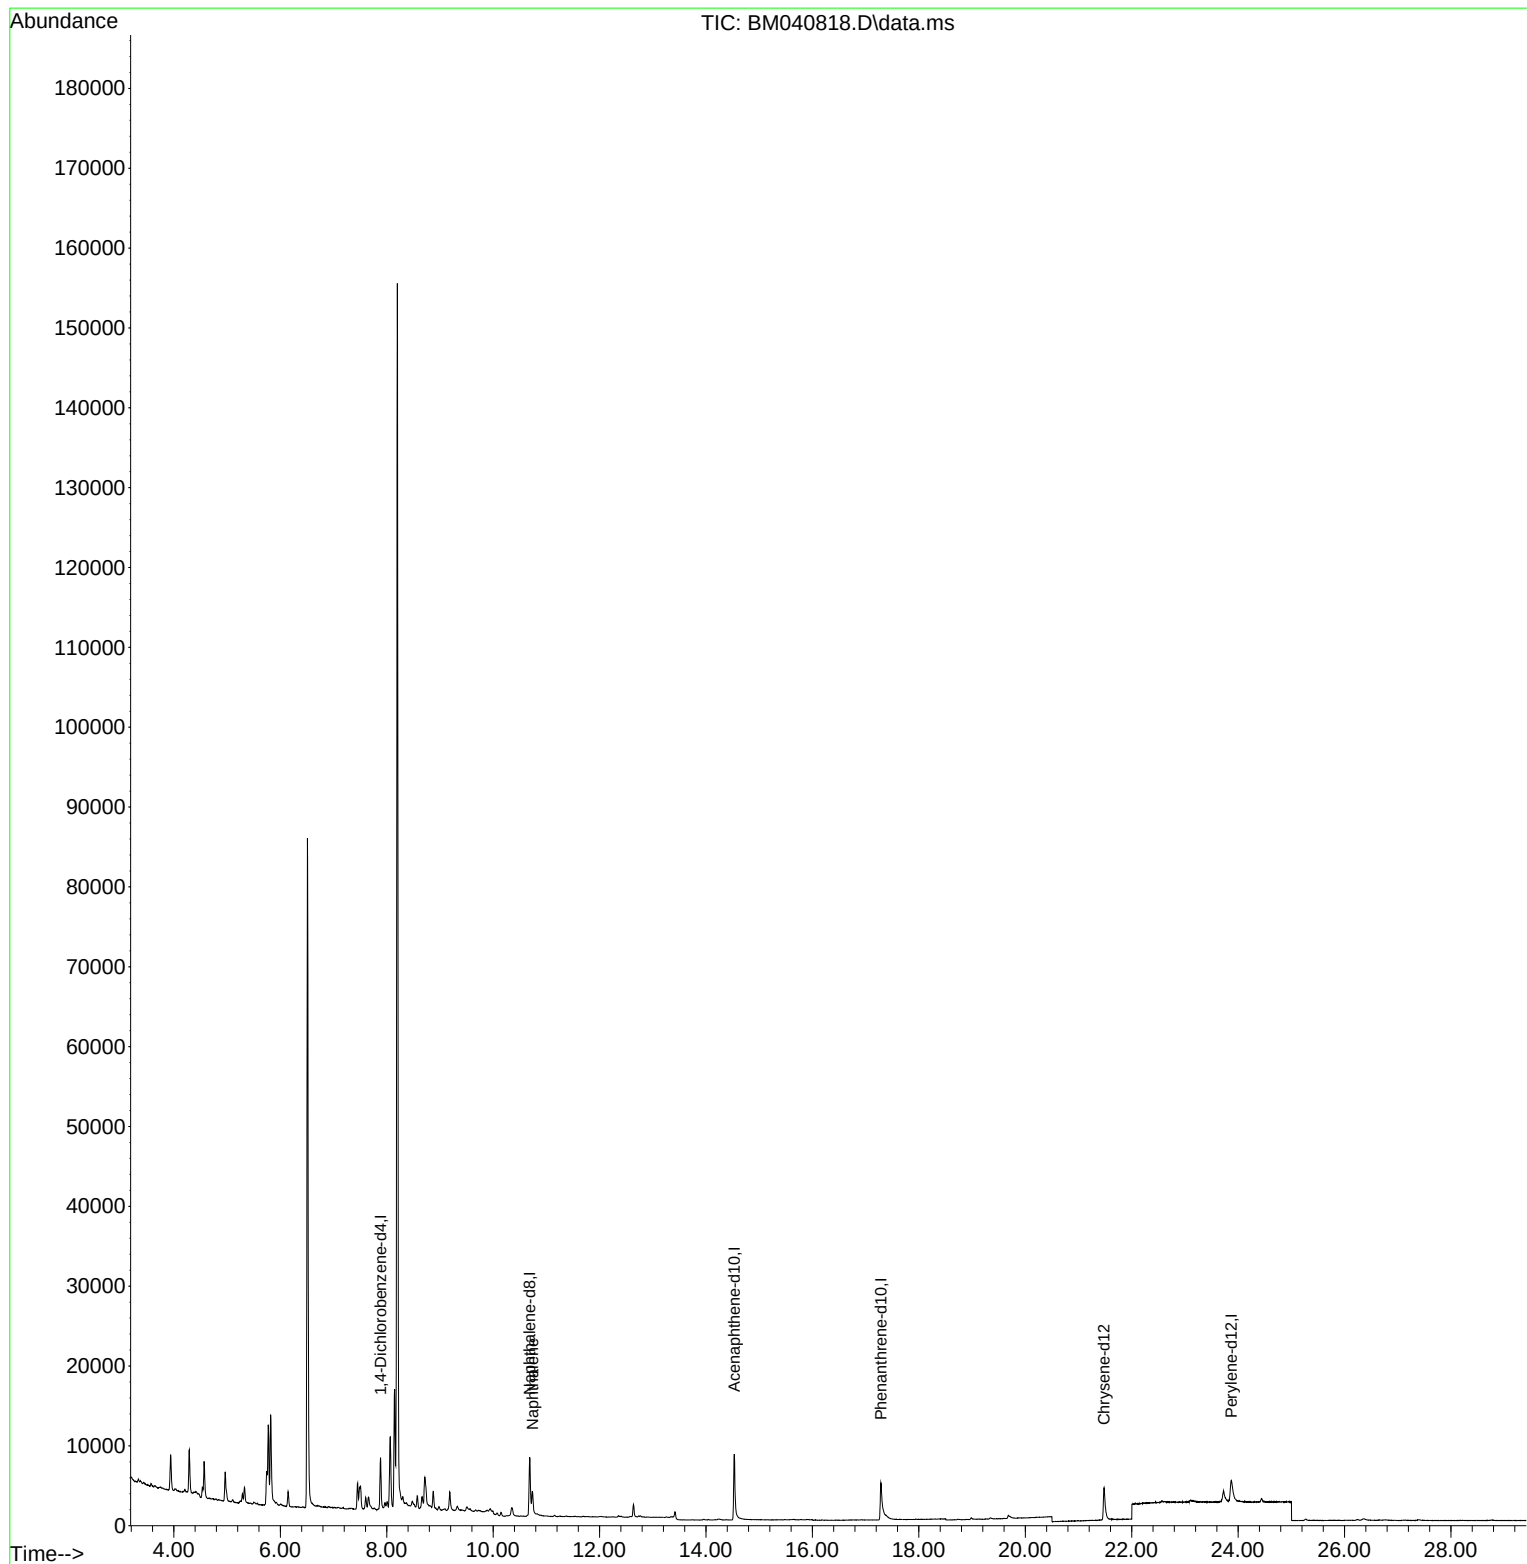

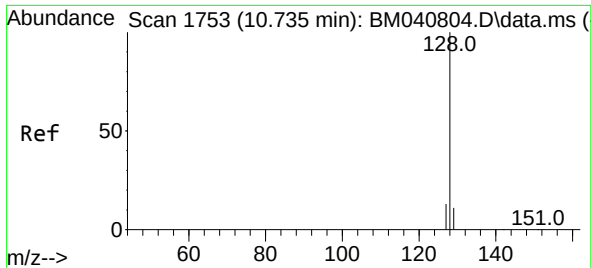

#5
Naphthalene
Concen: 0.133 ng/ul
RT: 10.740 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM040818.D
Acq: 11 Jul 2023 18:38

Instrument :
BNA_M
ClientSampleId :
SSTD0.4170

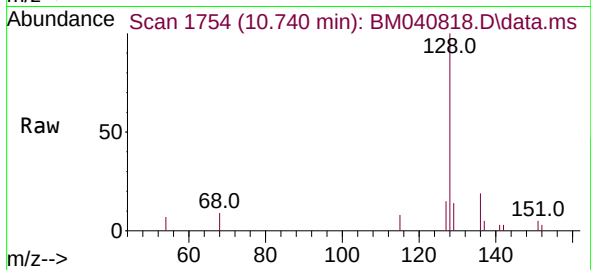

Tgt Ion:128 Resp: 4797
Ion Ratio Lower Upper
128 100
129 14.5 9.2 13.8#
127 14.9 10.6 15.8

