




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040808.D
 Acq On : 11 Jul 2023 12:11
 Operator : MA/JU
 Sample : 03477-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 HOA43

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

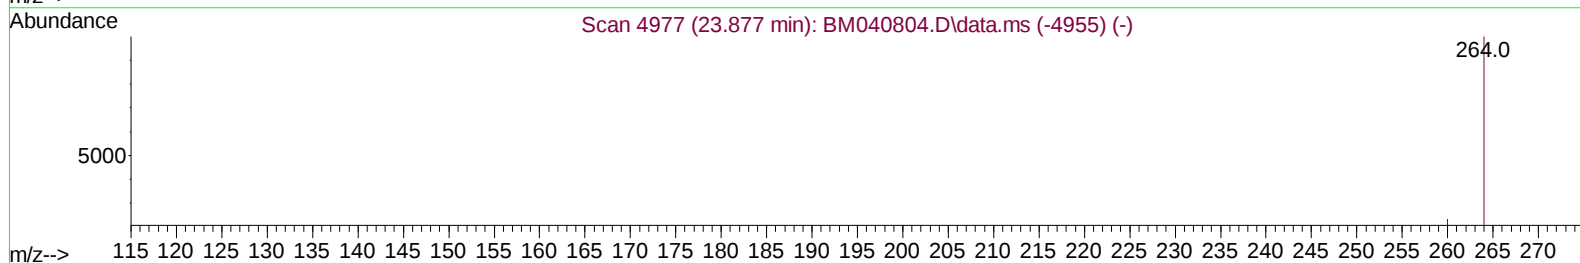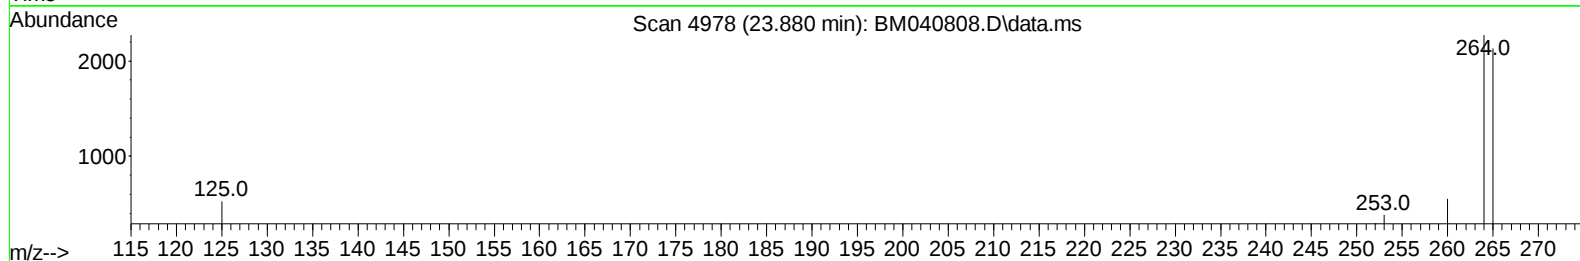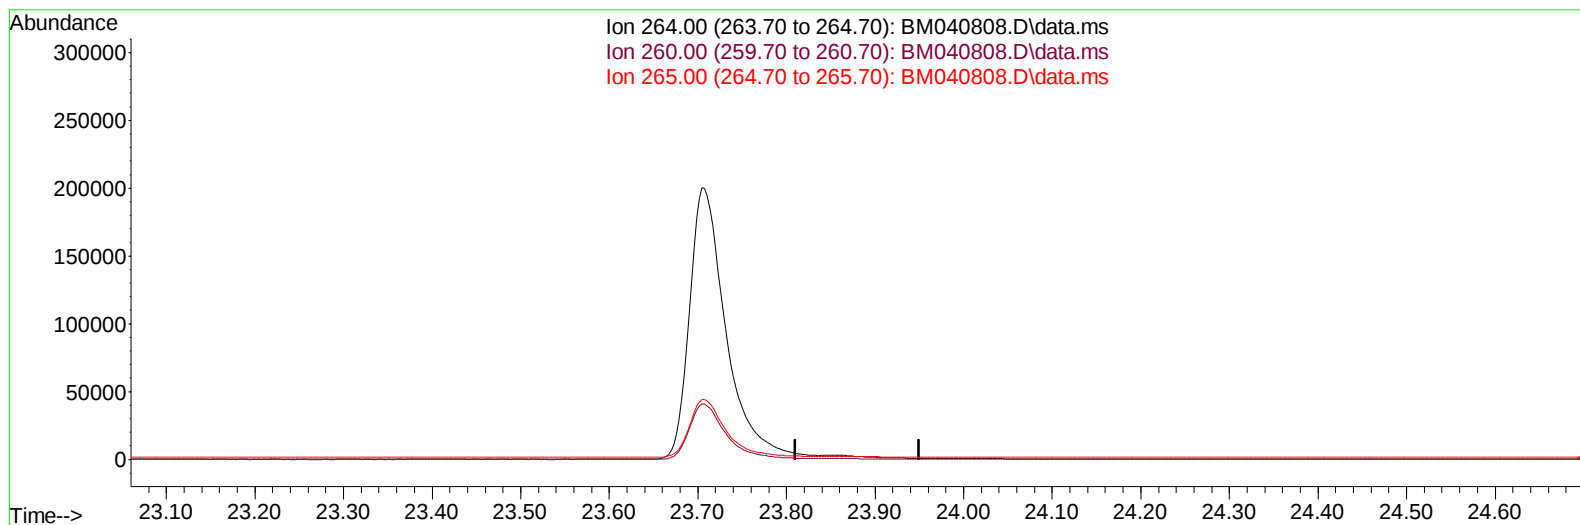

TIC: BM040808.D\data.ms

(23) Perylene-d12 (I)

23.880min (-23.880) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040808.D
 Acq On : 11 Jul 2023 12:11
 Operator : MA/JU
 Sample : 03477-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 HOA43

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

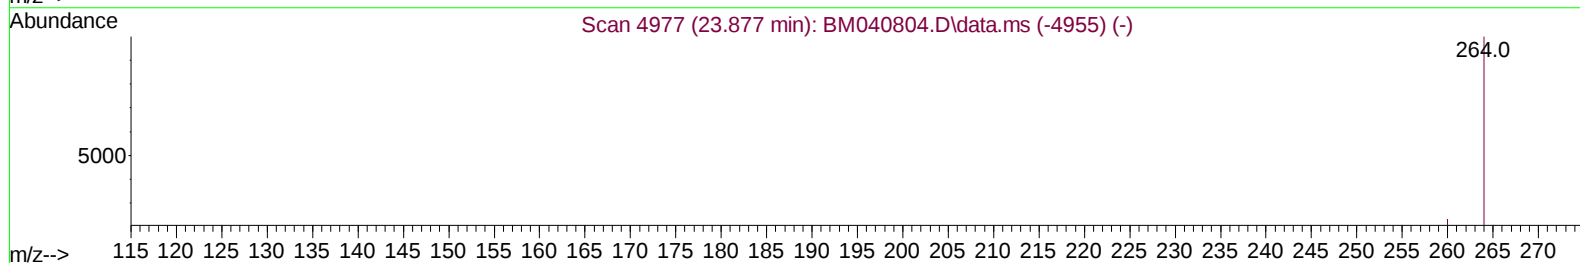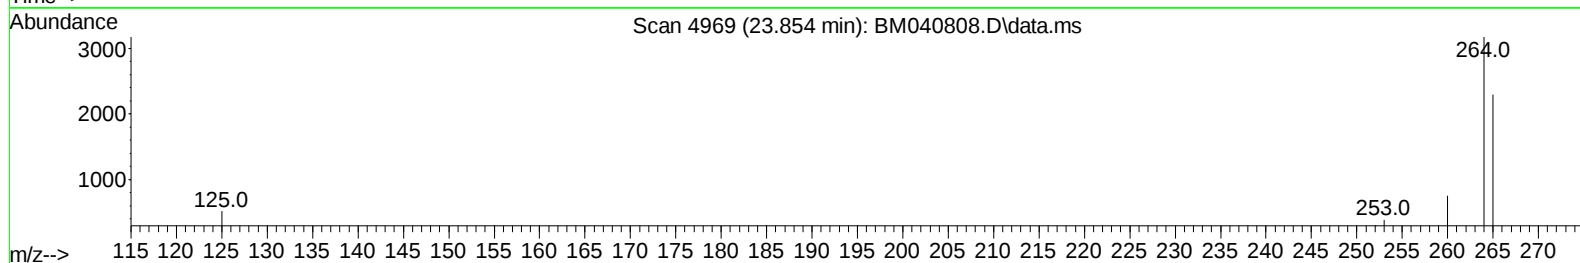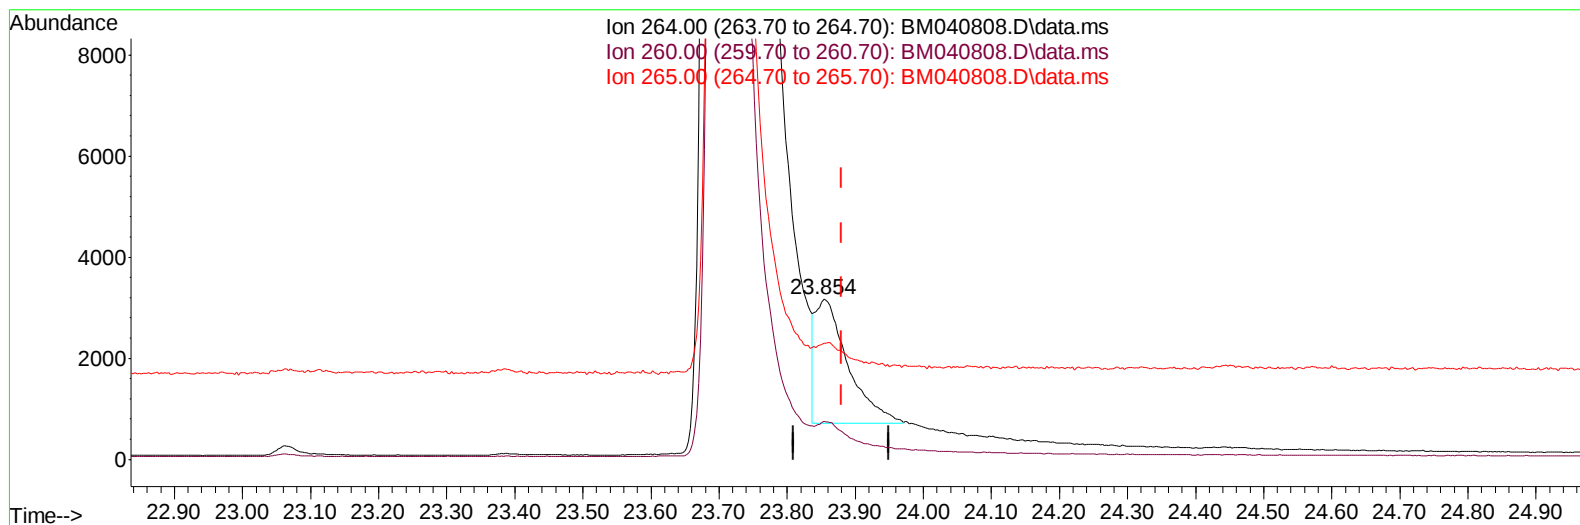

TIC: BM040808.D\data.ms

(23) Perylene-d12 (I)

23.854min (-0.026) 0.40 ng/ul m

response 8226

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.80
265.00	79.20	72.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040808.D
 Acq On : 11 Jul 2023 12:11
 Operator : MA/JU
 Sample : 03477-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 HOA43

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

Quant Time: Jul 12 04:33:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.878	152		2623	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136		9241	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164		4396	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188		7743	0.400	ng/ul	-0.01
17) Chrysene-d12	21.475	240		4586	0.400	ng/ul	-0.01
23) Perylene-d12	23.854	264		8226m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.296	96		24367	5.914	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.275	152		5310	0.410	ng/ul	-0.01
18) Fluoranthene-d10	19.306	212		8330	0.567	ng/ul	-0.01
Target Compounds							Qvalue
2) 1,4-Dioxane	3.330	88		399877	95.347	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040808.D
Acq On : 11 Jul 2023 12:11
Operator : MA/JU
Sample : 03477-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HOA43

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :mohammad ahmed 07/12/2023

