

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040809.D
Acq On : 11 Jul 2023 12:48
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HOA44

Quant Time: Jul 12 04:33:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Yogesh




Patel

07/12/2023

Supervised By :mohammad

ahmed

07/12/2023

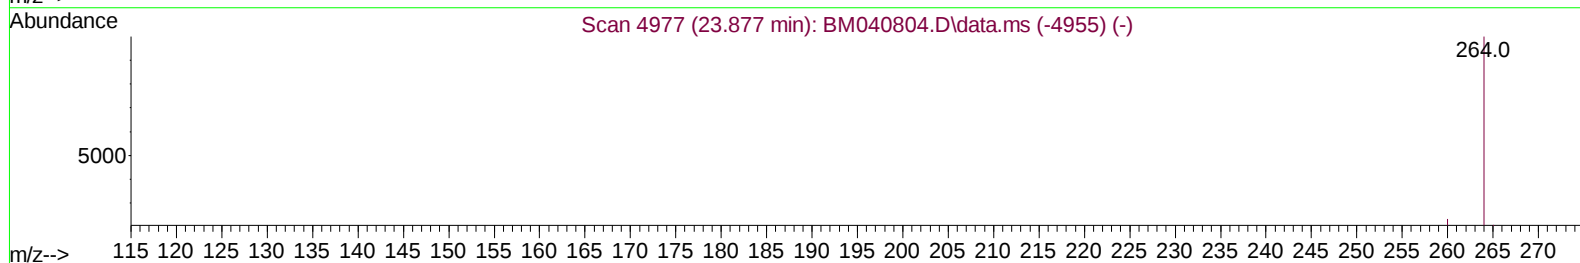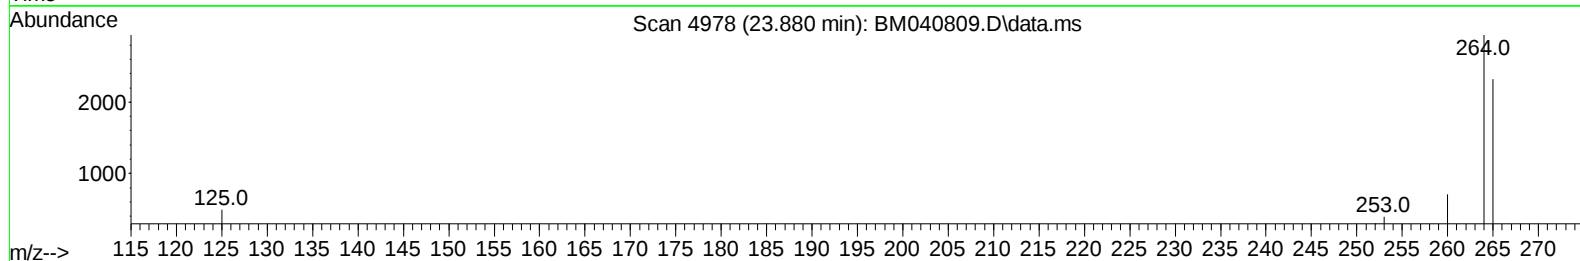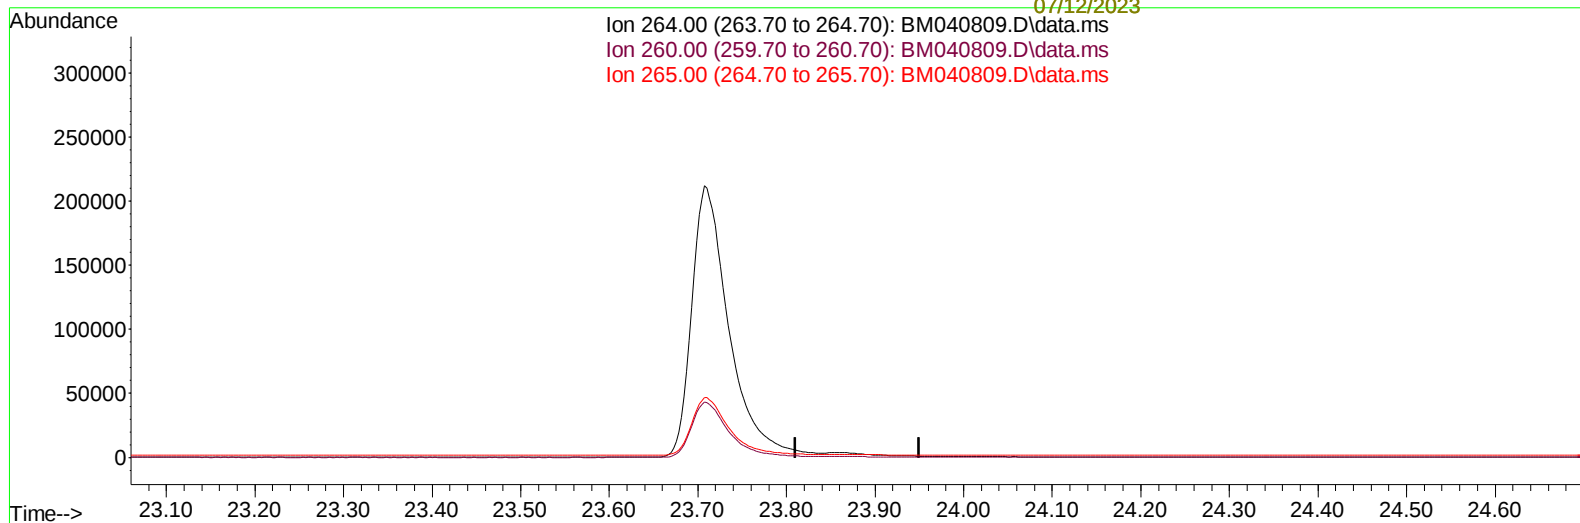

TIC: BM040809.D\data.ms

(23) Perylene-d12 (I)

23.880min (-23.880) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040809.D
Acq On : 11 Jul 2023 12:48
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HOA44

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

Reviewed By :Yogesh




Patel

07/12/2023

Supervised By :mohammad

ahmed

07/12/2023

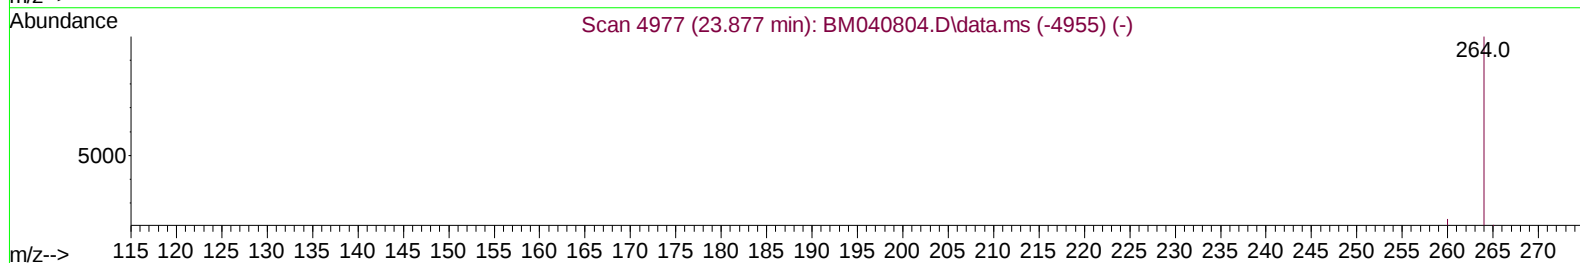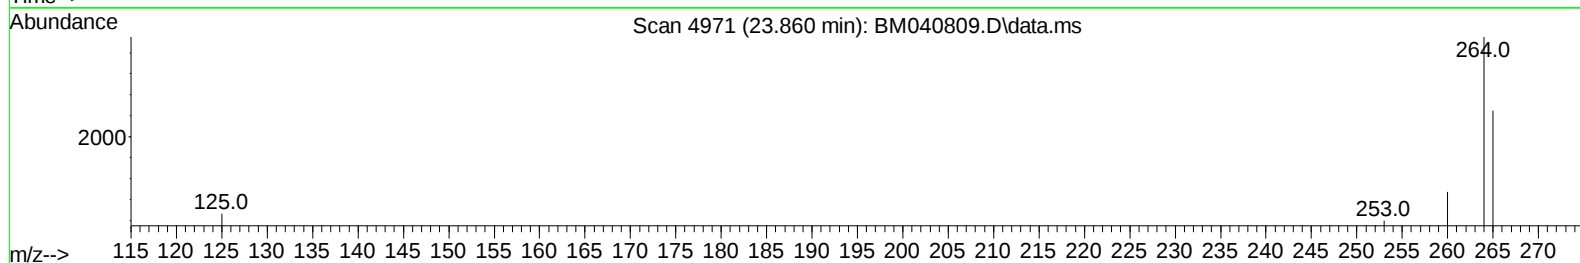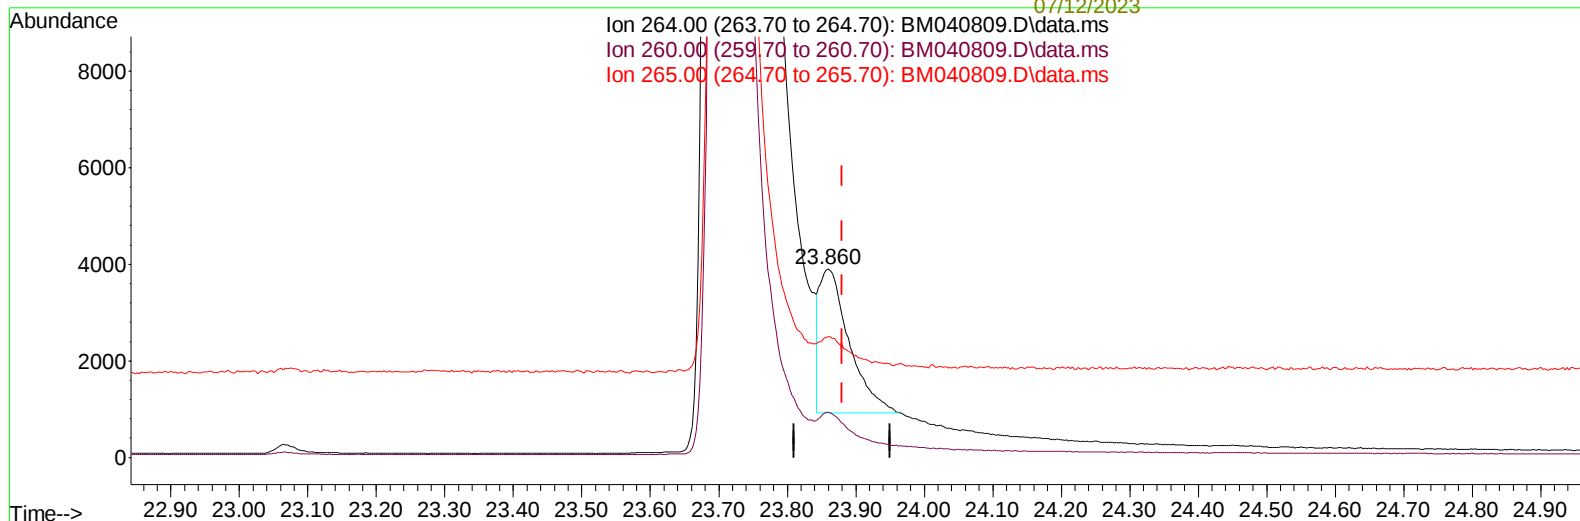

TIC: BM040809.D\data.ms

(23) Perylene-d12 (I)

23.860min (-0.020) 0.40 ng/ul m

response 9117

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	24.15
265.00	79.20	64.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040809.D
 Acq On : 11 Jul 2023 12:48
 Operator : MA/JU
 Sample : 03477-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 HOA44

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
 Patel
 07/12/2023

Supervised By :mohammad
 ahmed
 07/12/2023

Quant Time: Jul 12 04:33:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.882	152		3850	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136		13598	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164		6300	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188		10930	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240		6343	0.400	ng/ul	0.00
23) Perylene-d12	23.860	264		9117m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.296	96		26903	4.449	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152		5698	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.310	212		7589	0.373	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.330	88		438590	71.249	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040809.D
Acq On : 11 Jul 2023 12:48
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HOA44

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel
07/12/2023

Supervised By :mohammad
ahmed
07/12/2023

