




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040810.D
 Acq On : 11 Jul 2023 13:25
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

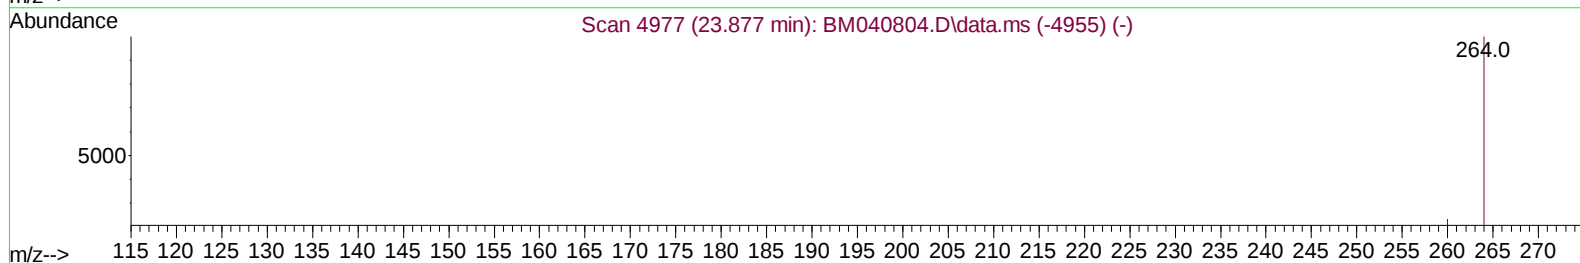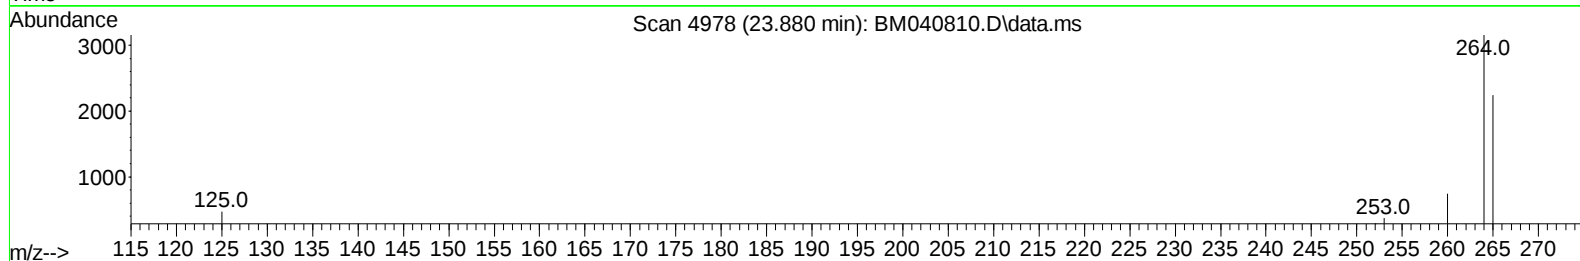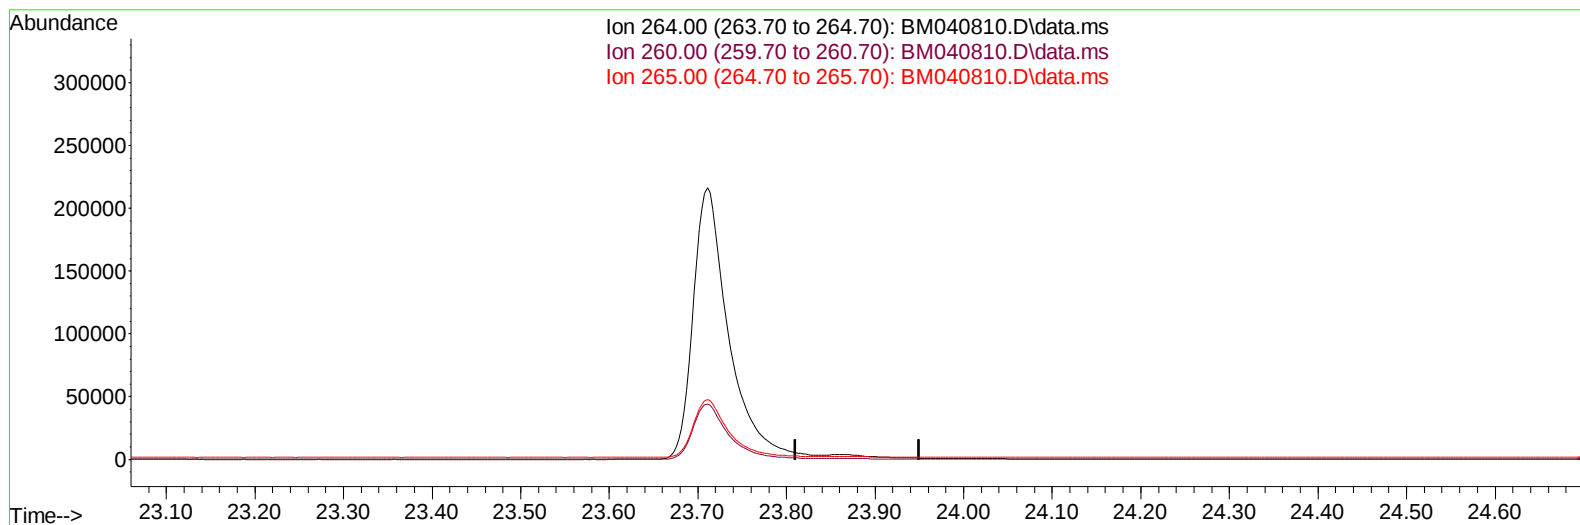

TIC: BM040810.D\data.ms

(23) Perylene-d12 (I)

23.880min (-23.880) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040810.D
 Acq On : 11 Jul 2023 13:25
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

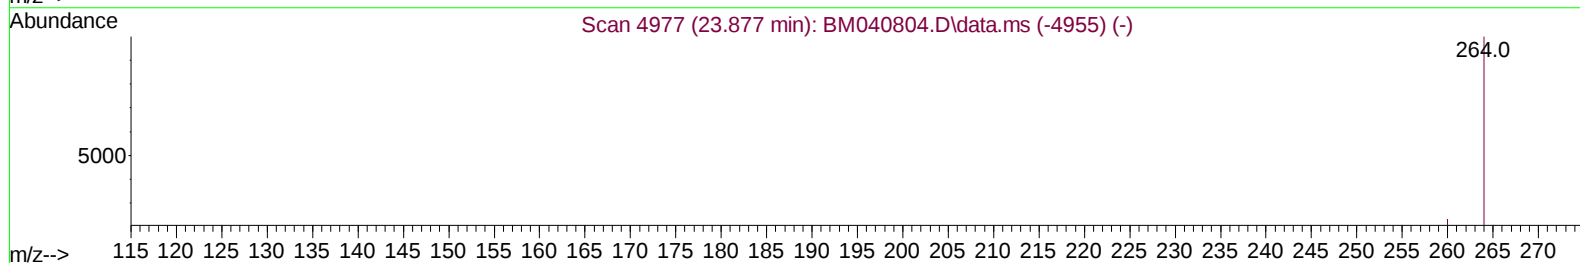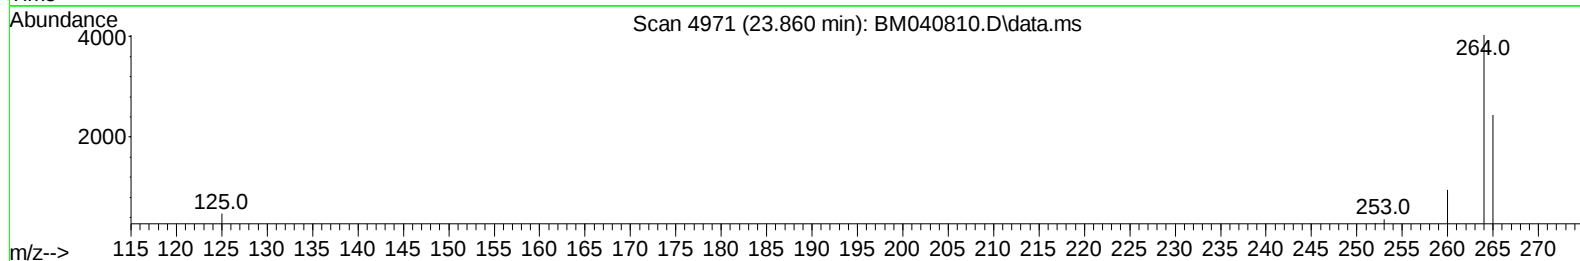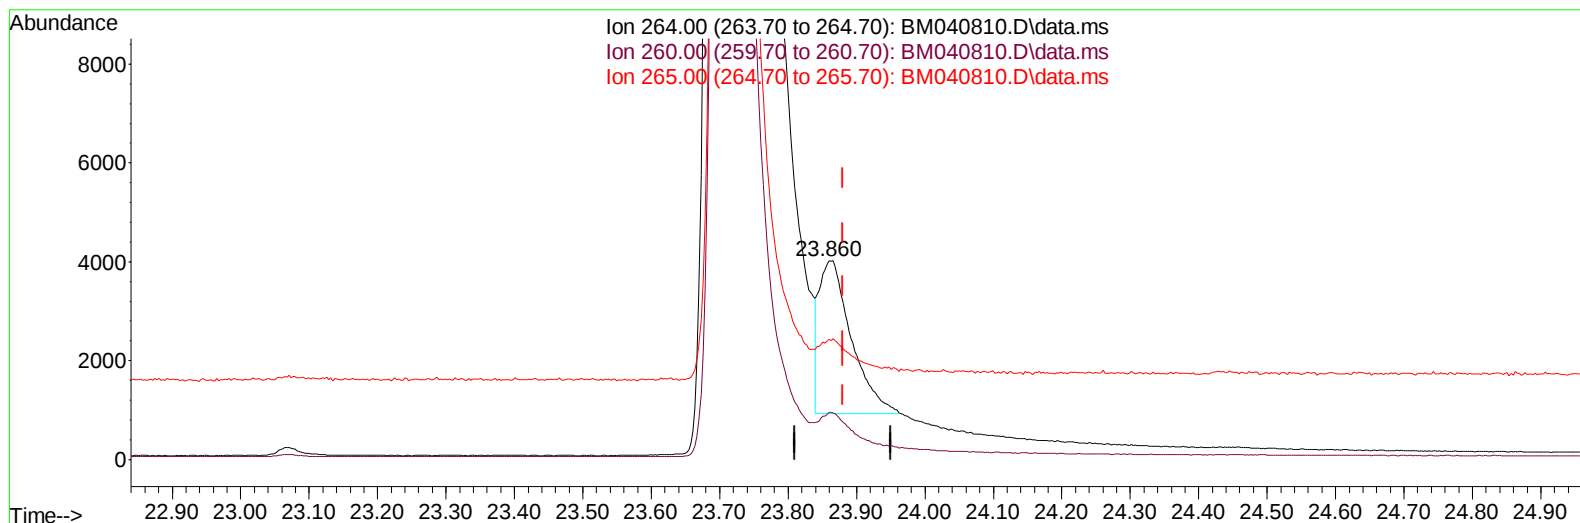

TIC: BM040810.D\data.ms

(23) Perylene-d12 (I)

23.860min (-0.020) 0.40 ng/ul m

response 10189

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.68
265.00	79.20	60.46#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040810.D
 Acq On : 11 Jul 2023 13:25
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

Quant Time: Jul 12 04:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 03:54:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.883	152	3942	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	13829	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	6845	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	12209	0.400	ng/ul	-0.01
17) Chrysene-d12	21.480	240	6965	0.400	ng/ul	0.00
23) Perylene-d12	23.860	264	10189m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	33112	5.347	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	5644	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.311	212	6791	0.304	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040810.D
Acq On : 11 Jul 2023 13:25
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 12 04:33:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 03:54:24 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :mohammad ahmed 07/12/2023

