




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040819.D
 Acq On : 11 Jul 2023 19:54
 Operator : MA/JU
 Sample : PB153941BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK941

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:37:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

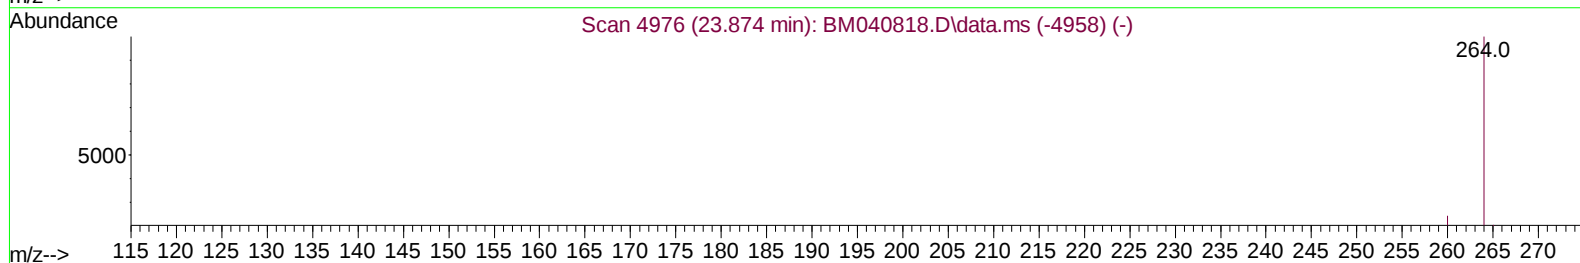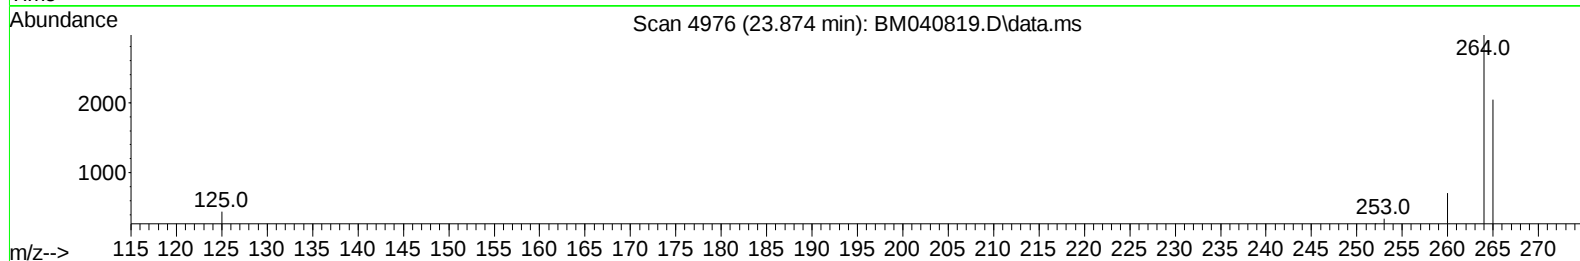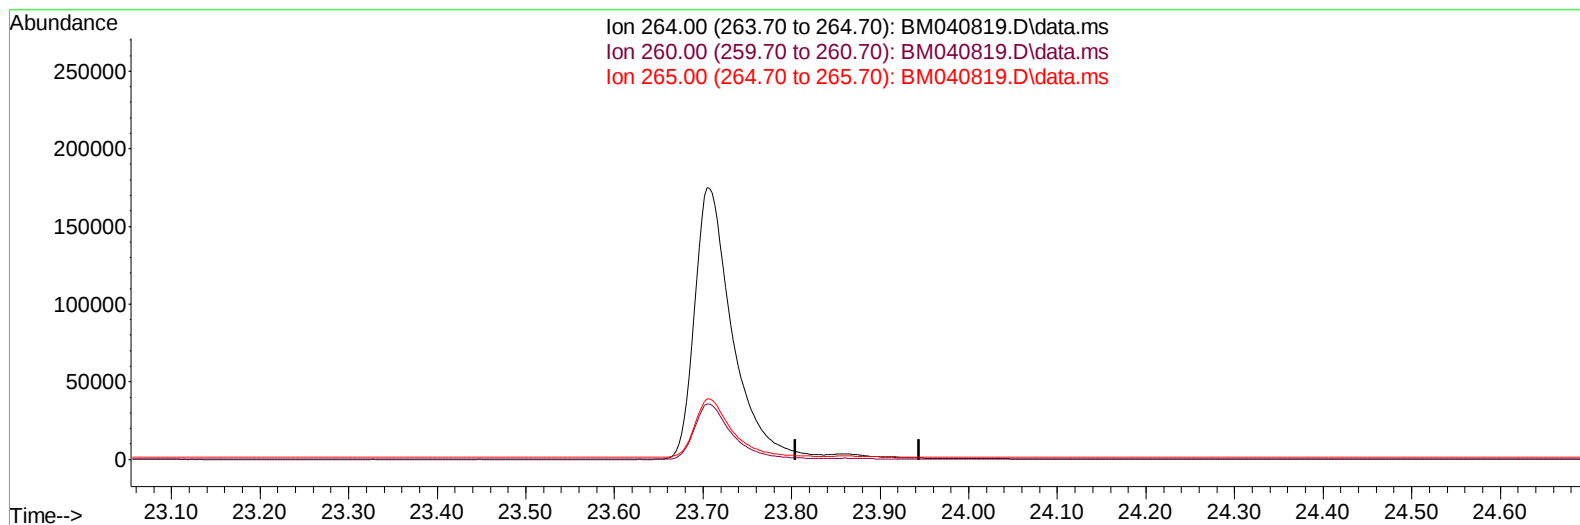

TIC: BM040819.D\data.ms

(23) Perylene-d12 (I)

23.874min (-23.874) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040819.D
 Acq On : 11 Jul 2023 19:54
 Operator : MA/JU
 Sample : PB153941BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK941

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:37:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

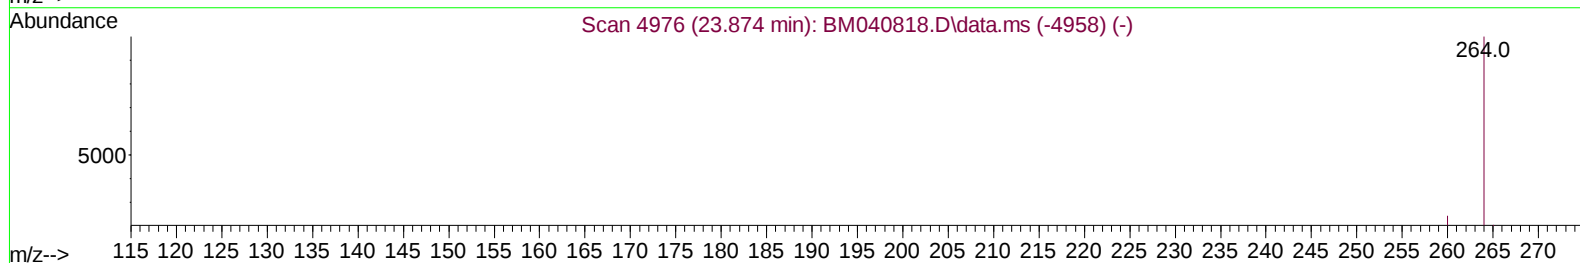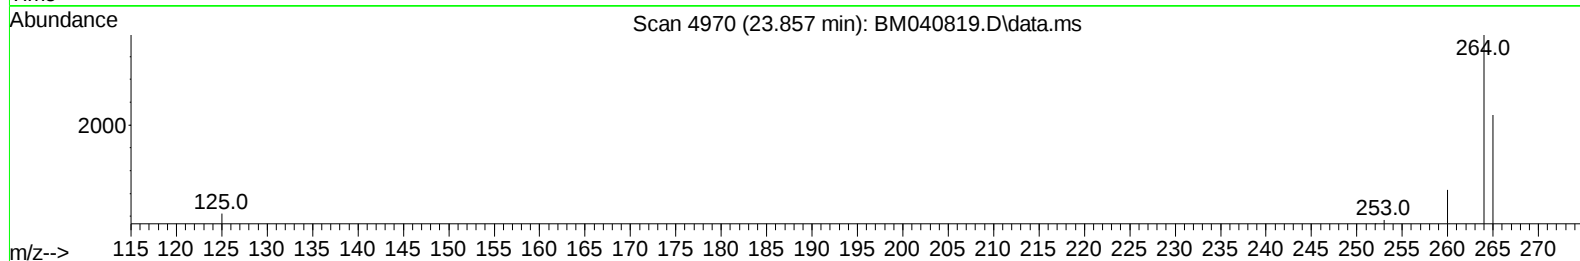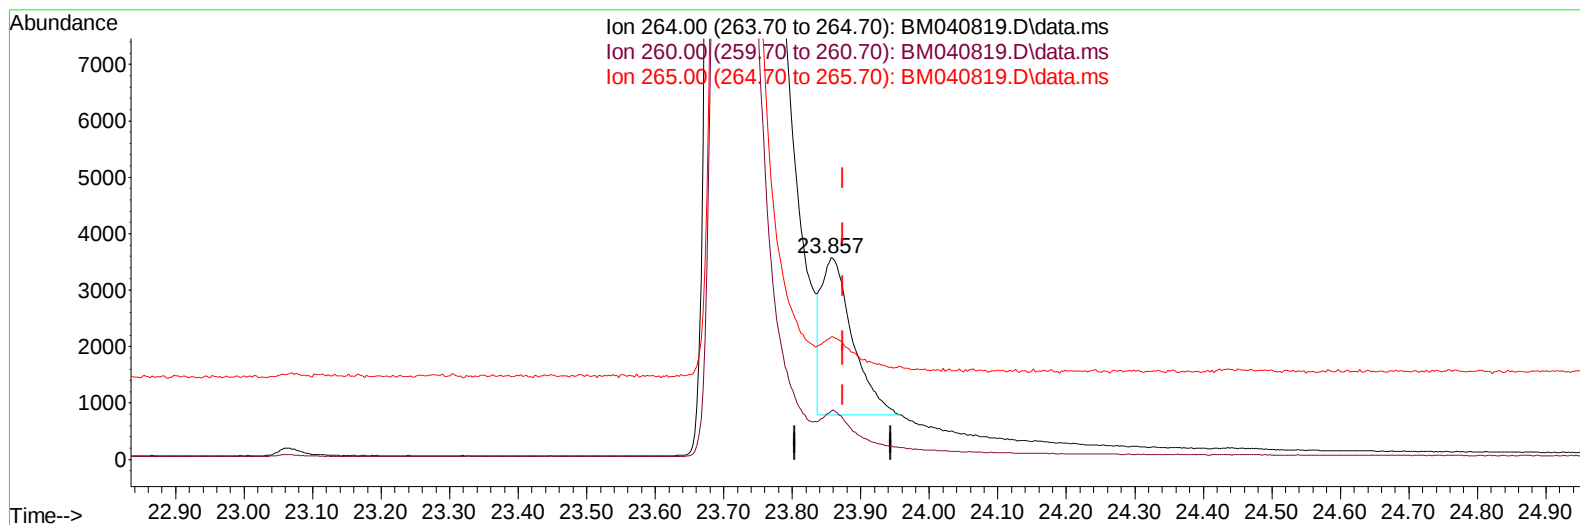

TIC: BM040819.D\data.ms

(23) Perylene-d12 (I)

23.857min (-0.018) 0.40 ng/ul m

response 8851

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	24.02
265.00	79.20	60.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040819.D
 Acq On : 11 Jul 2023 19:54
 Operator : MA/JU
 Sample : PB153941BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK941

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

Quant Time: Jul 12 05:37:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	3817	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	13730	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.527	164	6270	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.278	188	10413	0.400	ng/ul	-0.01
17) Chrysene-d12	21.474	240	6128	0.400	ng/ul	0.00
23) Perylene-d12	23.857	264	8851m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	33340	5.561	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152	5370	0.279	ng/ul	0.00
18) Fluoranthene-d10	19.310	212	5855	0.298	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040819.D
Acq On : 11 Jul 2023 19:54
Operator : MA/JU
Sample : PB153941BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK941

Manual IntegrationsAPPROVED

Quant Time: Jul 12 05:37:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :mohammad ahmed 07/12/2023

