

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071123\  
 Data File : BM040808.D  
 Acq On : 11 Jul 2023 12:11  
 Operator : MA/JU  
 Sample : 03477-05  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 HOA43

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 07/12/2023  
 Supervised By :mohammad ahmed 07/12/2023

Quant Time: Jul 12 04:33:18 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM062223.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jul 11 03:54:24 2023  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|--------|--------|----------|
| -----                       |        |      |          |        |        |          |
| Internal Standards          |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.878  | 152  | 2623     | 0.400  | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.686 | 136  | 9241     | 0.400  | ng/ul  | # 0.00   |
| 9) Acenaphthene-d10         | 14.527 | 164  | 4396     | 0.400  | ng/ul  | # 0.00   |
| 13) Phenanthrene-d10        | 17.278 | 188  | 7743     | 0.400  | ng/ul  | -0.01    |
| 17) Chrysene-d12            | 21.475 | 240  | 4586     | 0.400  | ng/ul  | -0.01    |
| 23) Perylene-d12            | 23.854 | 264  | 8226m    | 0.400  | ng/ul  | -0.03    |
|                             |        |      |          |        |        |          |
| System Monitoring Compounds |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8           | 3.296  | 96   | 24367    | 5.914  | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.275 | 152  | 5310     | 0.410  | ng/ul  | -0.01    |
| 18) Fluoranthene-d10        | 19.306 | 212  | 8330     | 0.567  | ng/ul  | -0.01    |
|                             |        |      |          |        |        |          |
| Target Compounds            |        |      |          |        |        | Qvalue   |
| 2) 1,4-Dioxane              | 3.330  | 88   | 399877   | 95.347 | ng/ul# | 84       |
| -----                       |        |      |          |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071123\  
Data File : BM040808.D  
Acq On : 11 Jul 2023 12:11  
Operator : MA/JU  
Sample : 03477-05  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
BNA\_M  
ClientSampleId :  
HOA43

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 07/12/2023  
Supervised By :mohammad ahmed 07/12/2023


Quant Time: Jul 12 04:33:18 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM062223.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 11 03:54:24 2023  
Response via : Initial Calibration

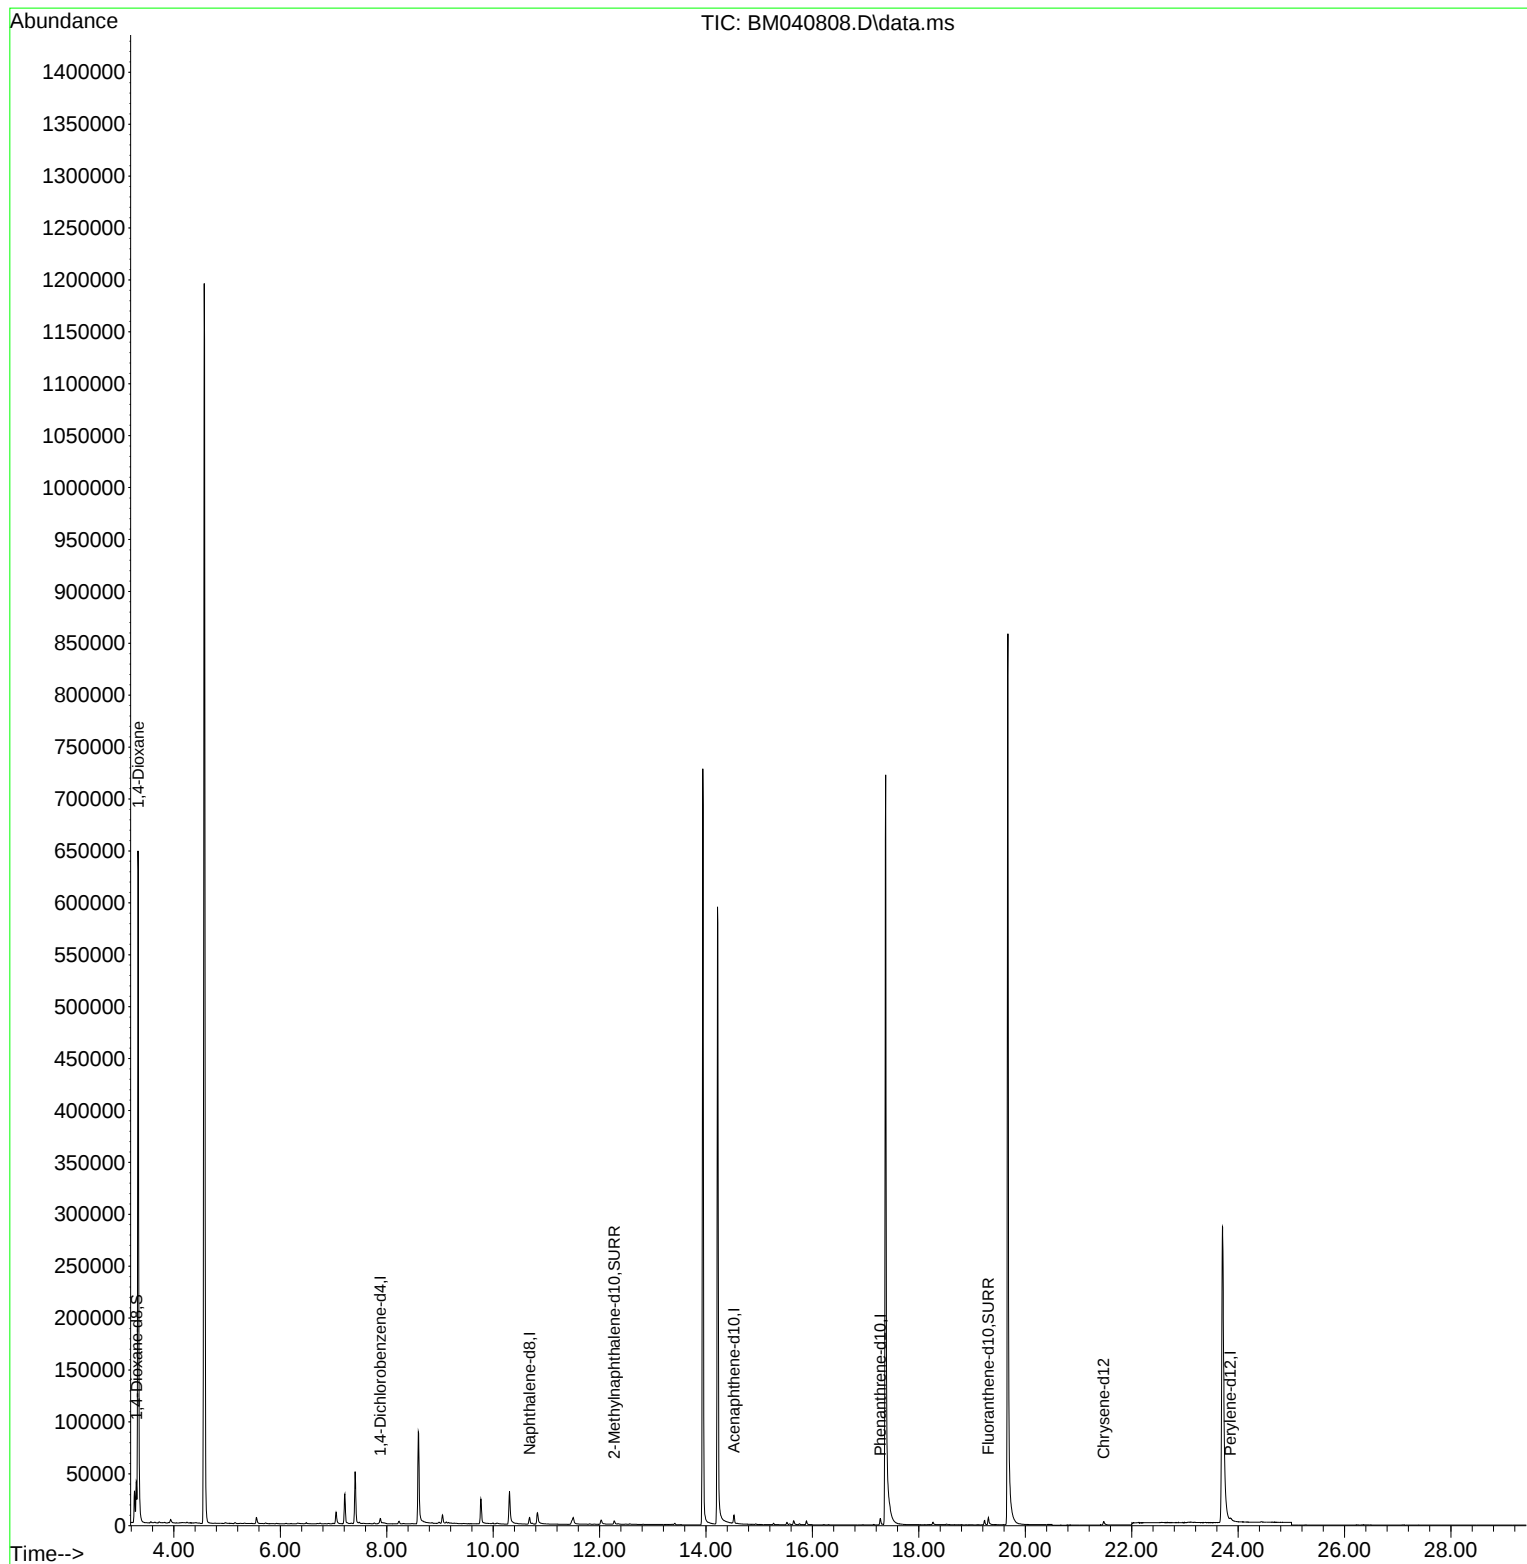

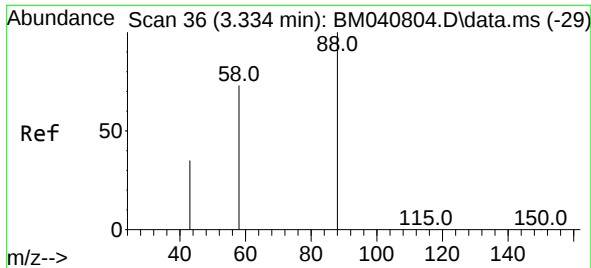

#2  
 1,4-Dioxane  
 Concen: 95.347 ng/ul  
 RT: 3.330 min Scan# 31  
 Delta R.T. -0.004 min  
 Lab File: BM040808.D  
 Acq: 11 Jul 2023 12:11

Instrument :  
 BNA\_M  
 ClientSampleId :  
 HOA43

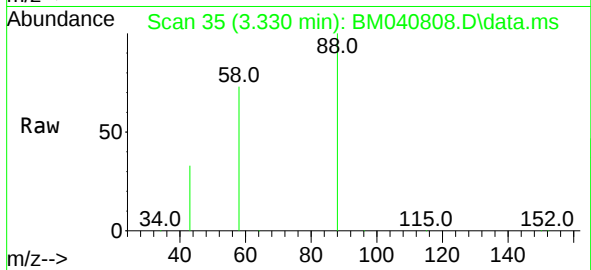

Tgt Ion: 88 Resp: 399872  
 Ion Ratio Lower Upper  
 88 100  
 43 32.6 36.1 54.1  
 58 72.9 49.8 74.8

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 07/12/2023  
 Supervised By :mohammad ahmed 07/12/2023

