

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
 Data File : BM040826.D
 Acq On : 12 Jul 2023 01:30
 Operator : MA/JU
 Sample : 03537-01DL 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH312DL

Quant Time: Jul 12 06:11:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.883	152	4038	0.400	ng/ul	0.00
4) Naphthalene-d8	10.686	136	14953	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.523	164	6567	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.278	188	9626	0.400	ng/ul	-0.01
17) Chrysene-d12	21.477	240	6438	0.400	ng/ul	0.00
23) Perylene-d12	23.863	264	5446	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	5790	0.913	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	1146	0.055	ng/ul	0.00
18) Fluoranthene-d10	19.311	212	1314	0.064	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.334	88	877	0.136	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071123\
Data File : BM040826.D
Acq On : 12 Jul 2023 01:30
Operator : MA/JU
Sample : 03537-01DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH312DL

Quant Time: Jul 12 06:11:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

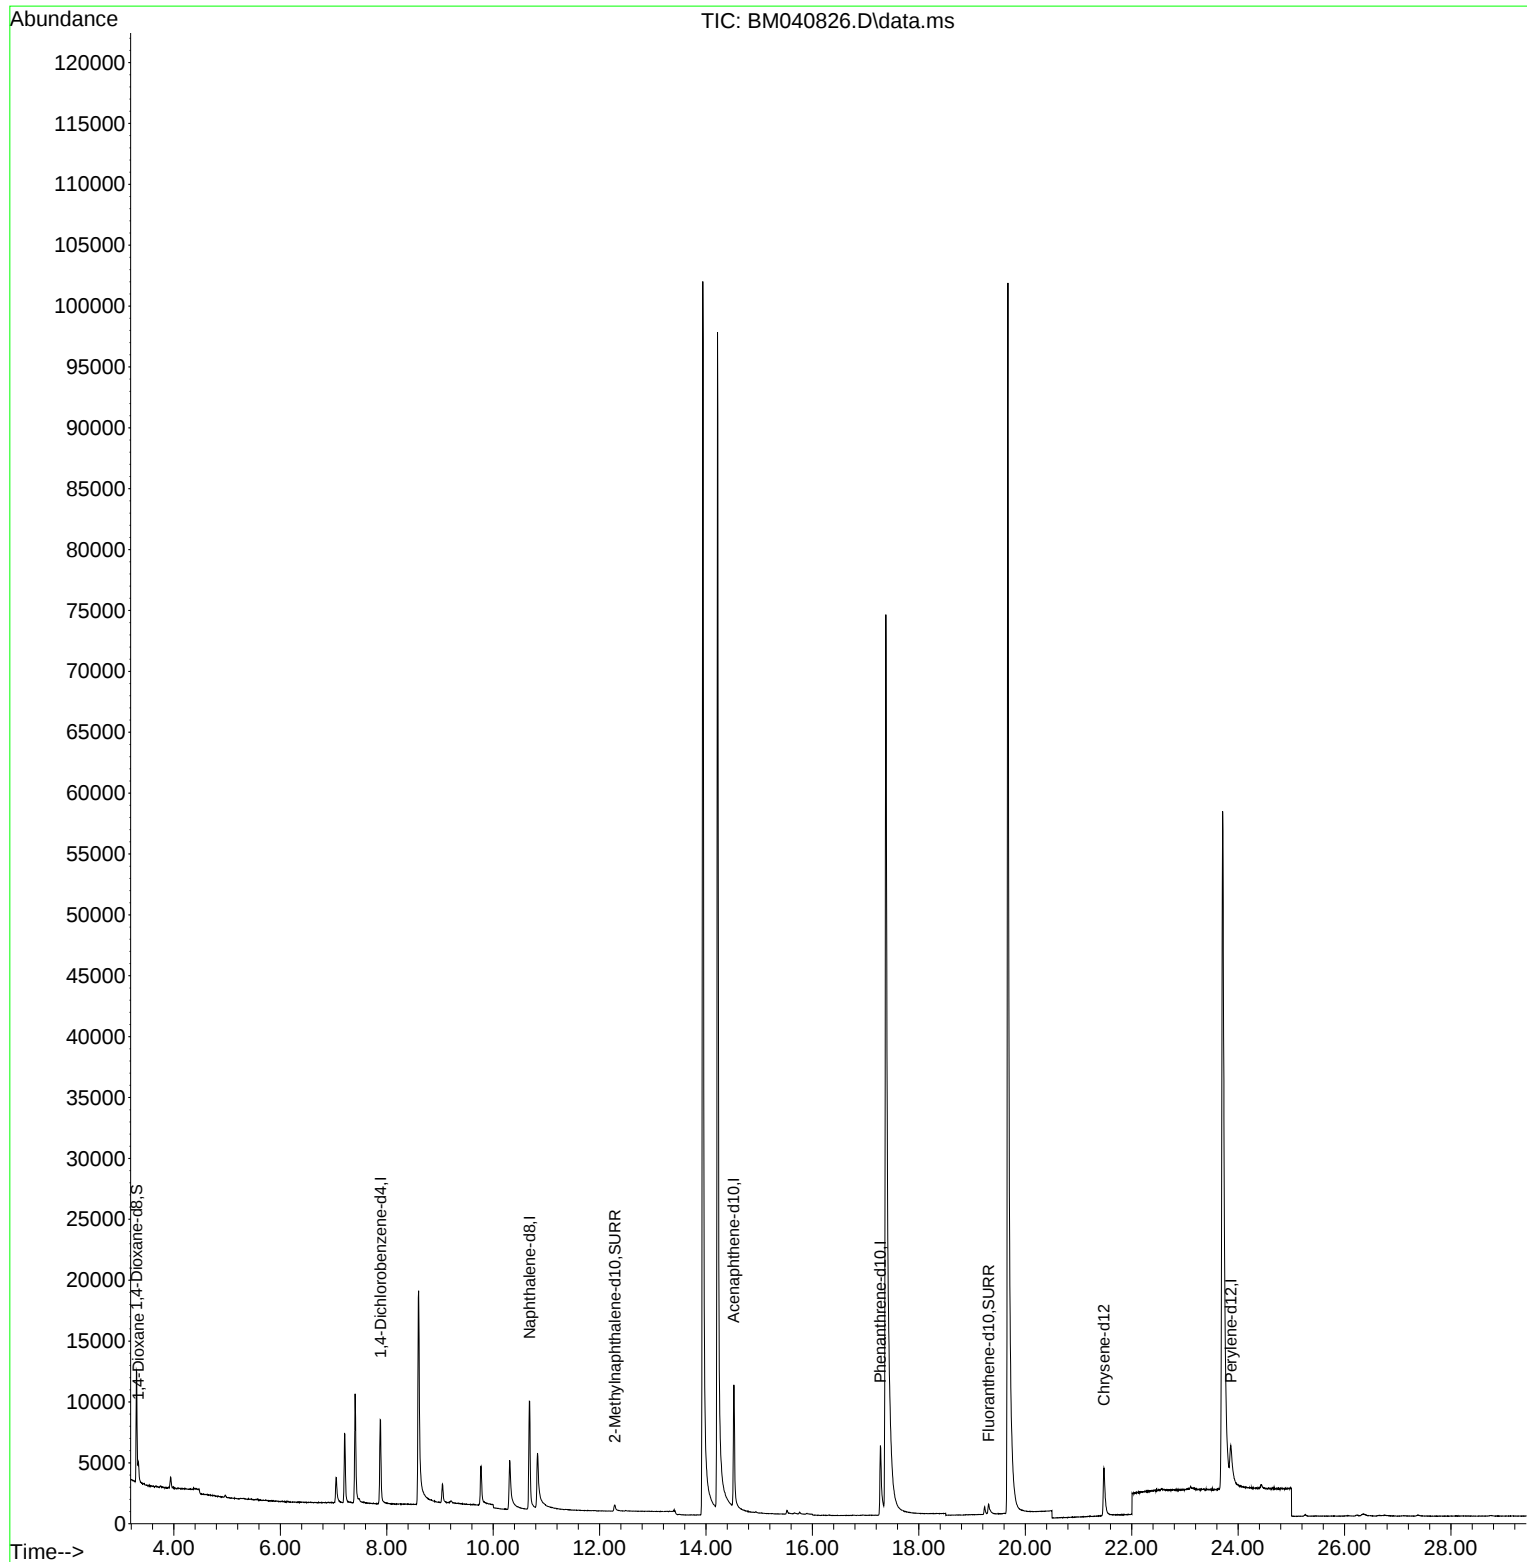

Abundance Scan 36 (3.334 min): BM040818.D\data.ms (-29)

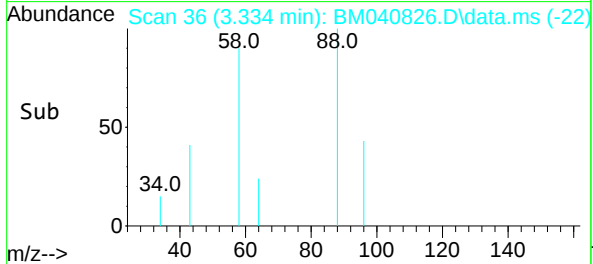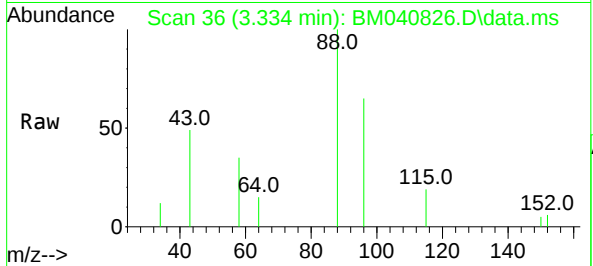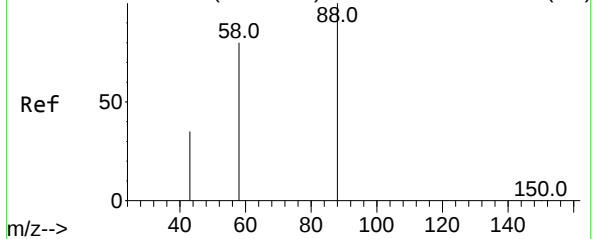

#2
1,4-Dioxane
Concen: 0.136 ng/ul
RT: 3.334 min Scan# 30
Delta R.T. 0.000 min
Lab File: BM040826.D
Acq: 12 Jul 2023 01:30

Instrument :
BNA_M
ClientSampleId :
BH312DL

Tgt Ion:	88	Resp:	877
Ion	Ratio	Lower	Upper
88	100		
43	49.5	36.1	54.1
58	34.8	49.8	74.8

