
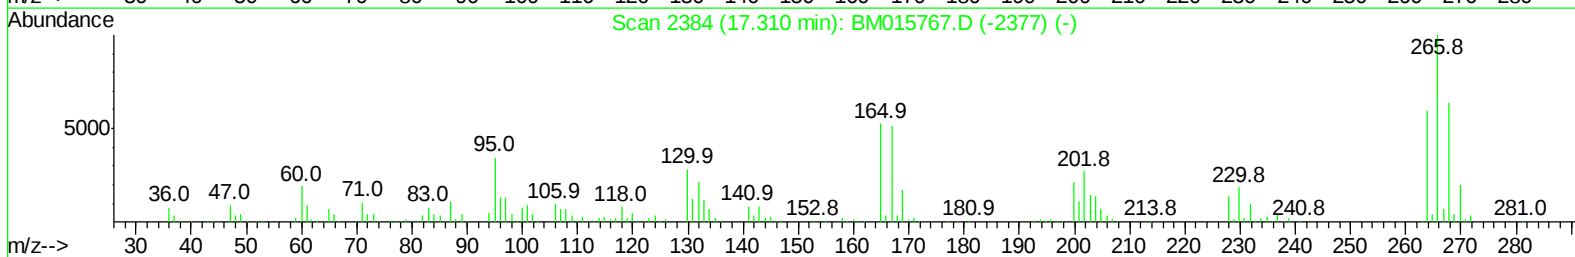
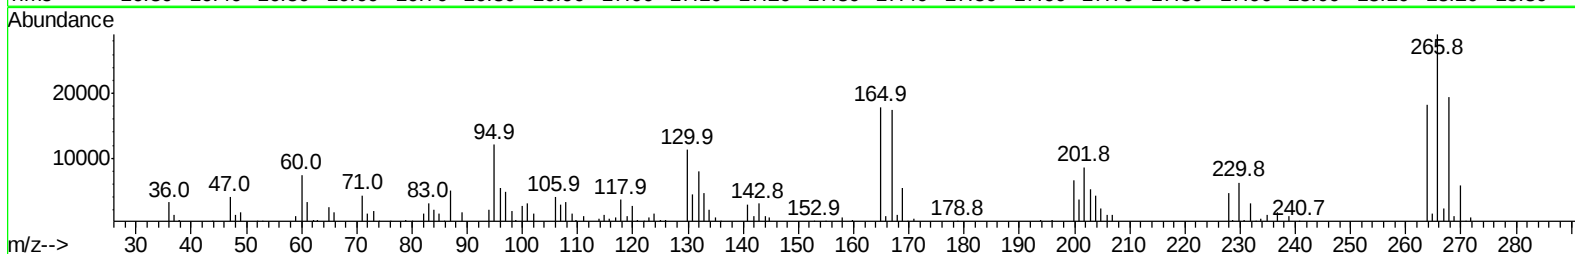


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071218\
Data File : BM015917.D
Acq On : 12 Jul 2018 16:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 07:50:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

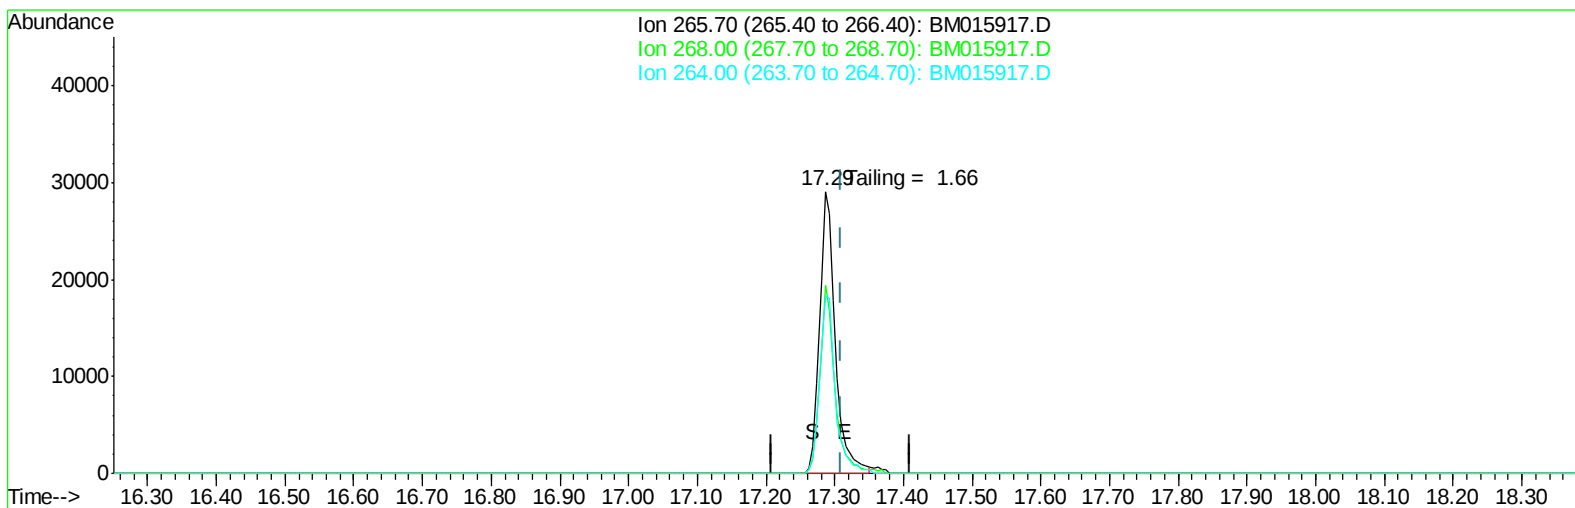

TIC: BM015917.D

(69) Pentachlorophenol (C)




17.286min (-0.024) 0.00ng

response 46910

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	66.82
264.00	61.20	62.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071218\
Data File : BM015917.D
Acq On : 12 Jul 2018 16:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 07:50:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

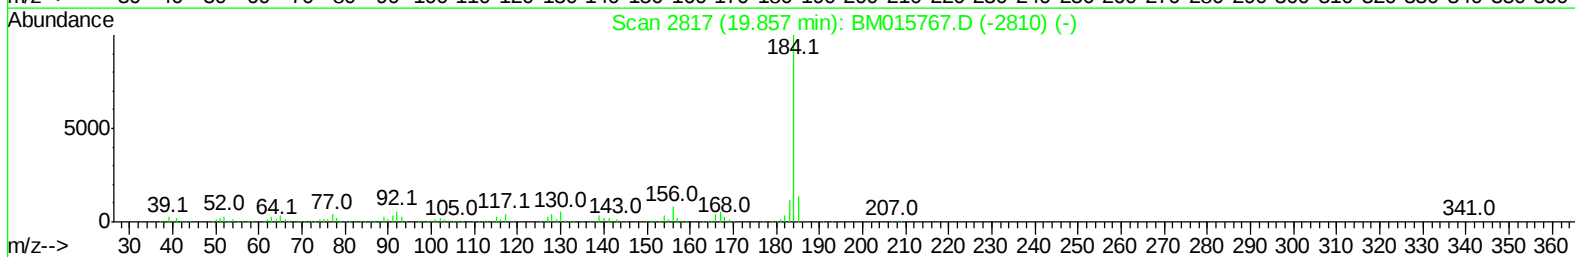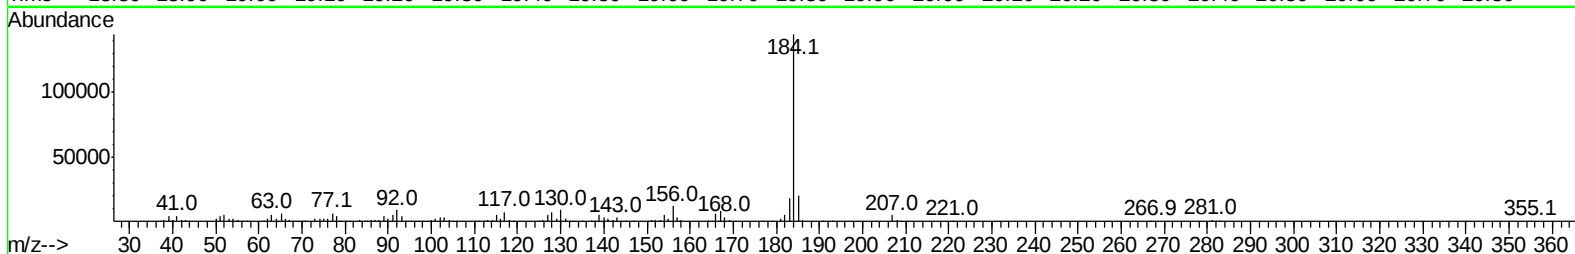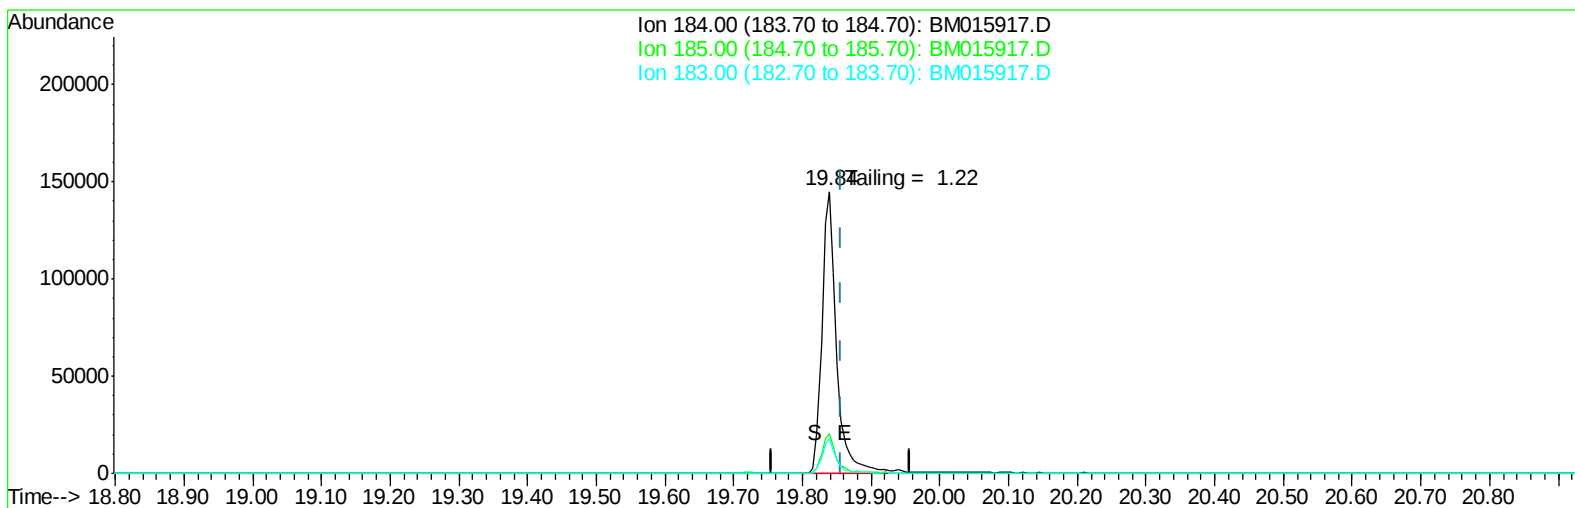

TIC: BM015917.D

(76) Benzidine

19.839min (-0.018) 11546.58ng

response 214822

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.01
183.00	11.10	12.39
0.00	0.00	0.00