


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071218\
Data File : BM015917.D
Acq On : 12 Jul 2018 16:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 05 17:39:50 2018

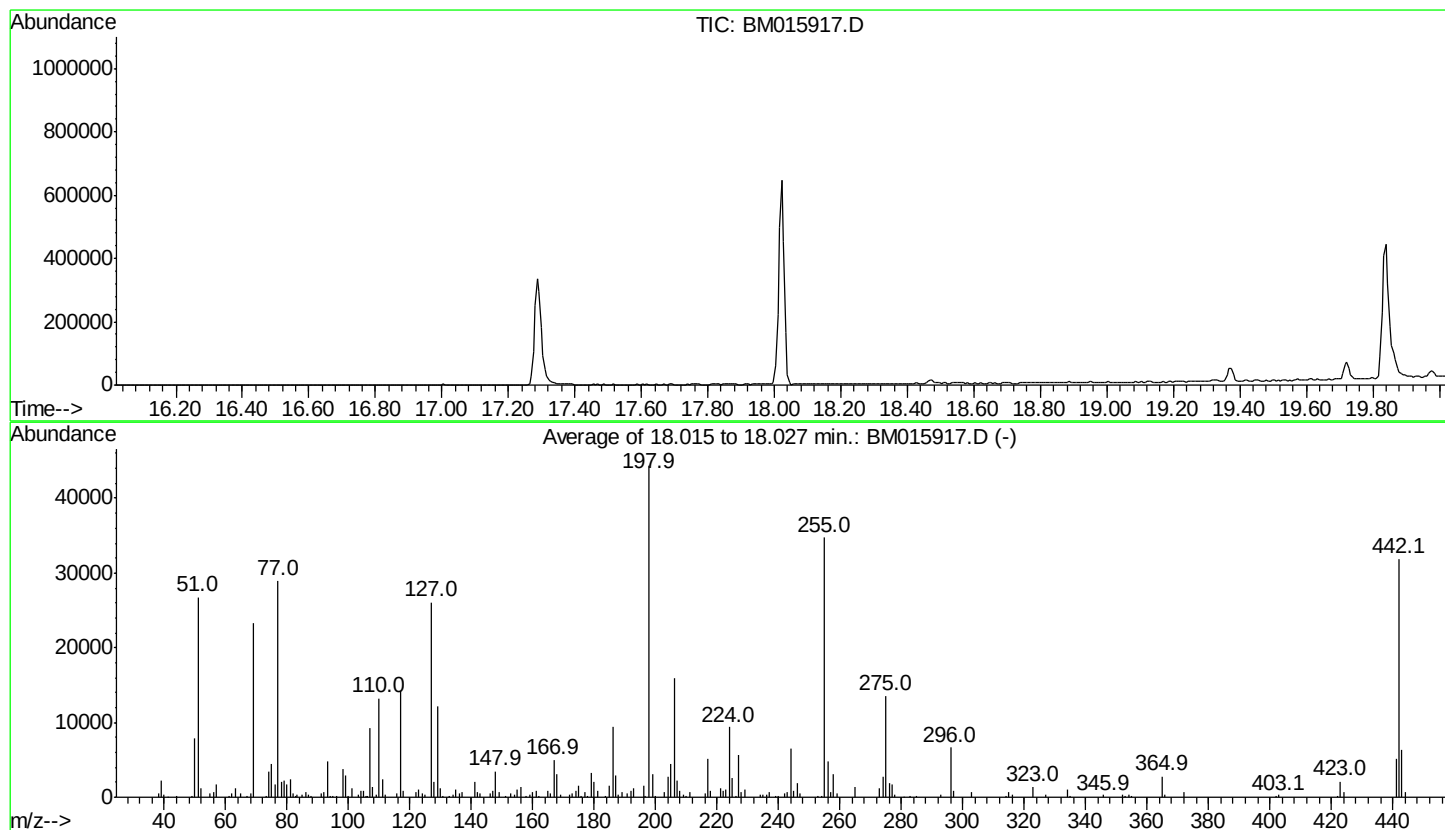

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.4	26794	PASS
68	69	0.00	2	1.9	436	PASS
69	198	0.00	100	52.4	23237	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.8	26104	PASS
197	198	0.00	2	0.2	101	PASS
198	198	100	100	100.0	44368	PASS
199	198	5	9	6.9	3075	PASS
275	198	10	60	30.6	13571	PASS
365	198	1	100	6.3	2789	PASS
441	443	0.01	100	80.1	5080	PASS
442	198	50	100	72.0	31933	PASS
443	442	15	24	19.9	6341	PASS