

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040832.D
 Acq On : 12 Jul 2023 11:40
 Operator : MA/JU
 Sample : 03414-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4646

Quant Time: Jul 13 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	4518	0.400	ng/ul	0.00
4) Naphthalene-d8	10.680	136	17726	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.527	164	8095	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.282	188	13047	0.400	ng/ul	0.00
17) Chrysene-d12	21.474	240	9177	0.400	ng/ul	0.00
23) Perylene-d12	23.865	264	7322	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.313	96	61	0.009	ng/ul	0.01
6) 2-Methylnaphthalene-d10	12.275	152	3963	0.159	ng/ul	-0.01
18) Fluoranthene-d10	19.310	212	5468	0.186	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.730	128	6621	0.135	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040832.D
Acq On : 12 Jul 2023 11:40
Operator : MA/JU
Sample : 03414-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4646


Quant Time: Jul 13 00:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

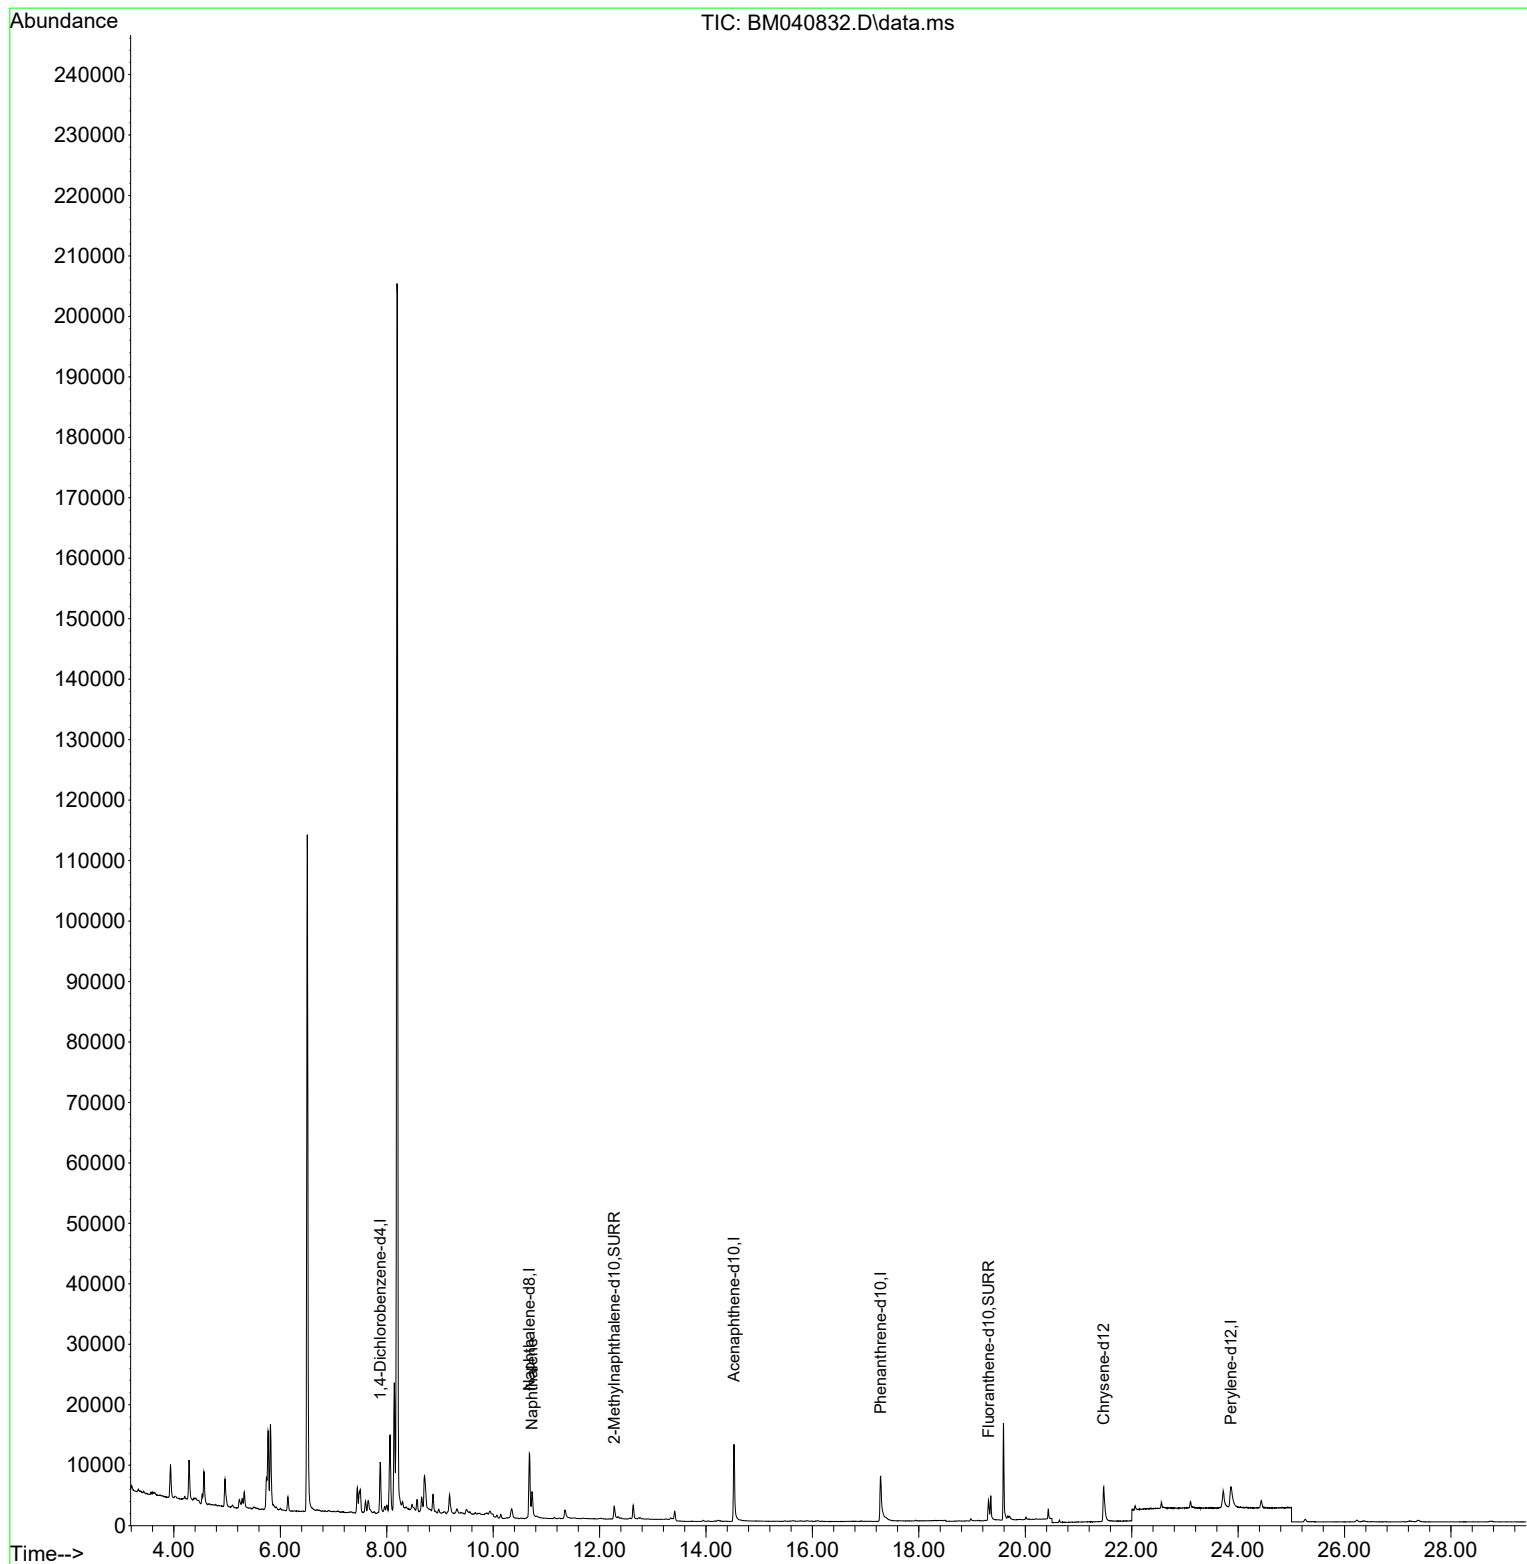

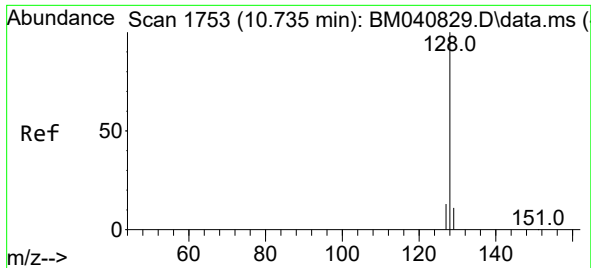

#5
Naphthalene
Concen: 0.135 ng/ul
RT: 10.730 min Scan# 11
Delta R.T. -0.011 min
Lab File: BM040832.D
Acq: 12 Jul 2023 11:40

Instrument :
BNA_M
ClientSampleId :
A4646

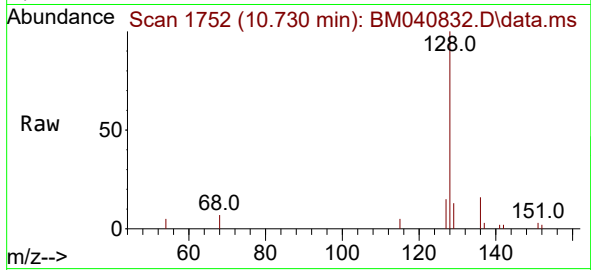

Tgt Ion:	128	Resp:	6621
Ion	Ratio	Lower	Upper
128	100		
129	13.1	9.2	13.8
127	14.6	10.6	15.8

