

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040833.D
 Acq On : 12 Jul 2023 12:18
 Operator : MA/JU
 Sample : 03414-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46G4

Quant Time: Jul 13 00:12:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	3912	0.400	ng/ul	0.00
4) Naphthalene-d8	10.680	136	15095	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.527	164	7001	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.282	188	10967	0.400	ng/ul	0.00
17) Chrysene-d12	21.474	240	7294	0.400	ng/ul	0.00
23) Perylene-d12	23.865	264	5267	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	993	0.162	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.275	152	3831	0.181	ng/ul	-0.01
18) Fluoranthene-d10	19.310	212	4892	0.209	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.735	128	6616	0.159	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040833.D
Acq On : 12 Jul 2023 12:18
Operator : MA/JU
Sample : 03414-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46G4


Quant Time: Jul 13 00:12:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

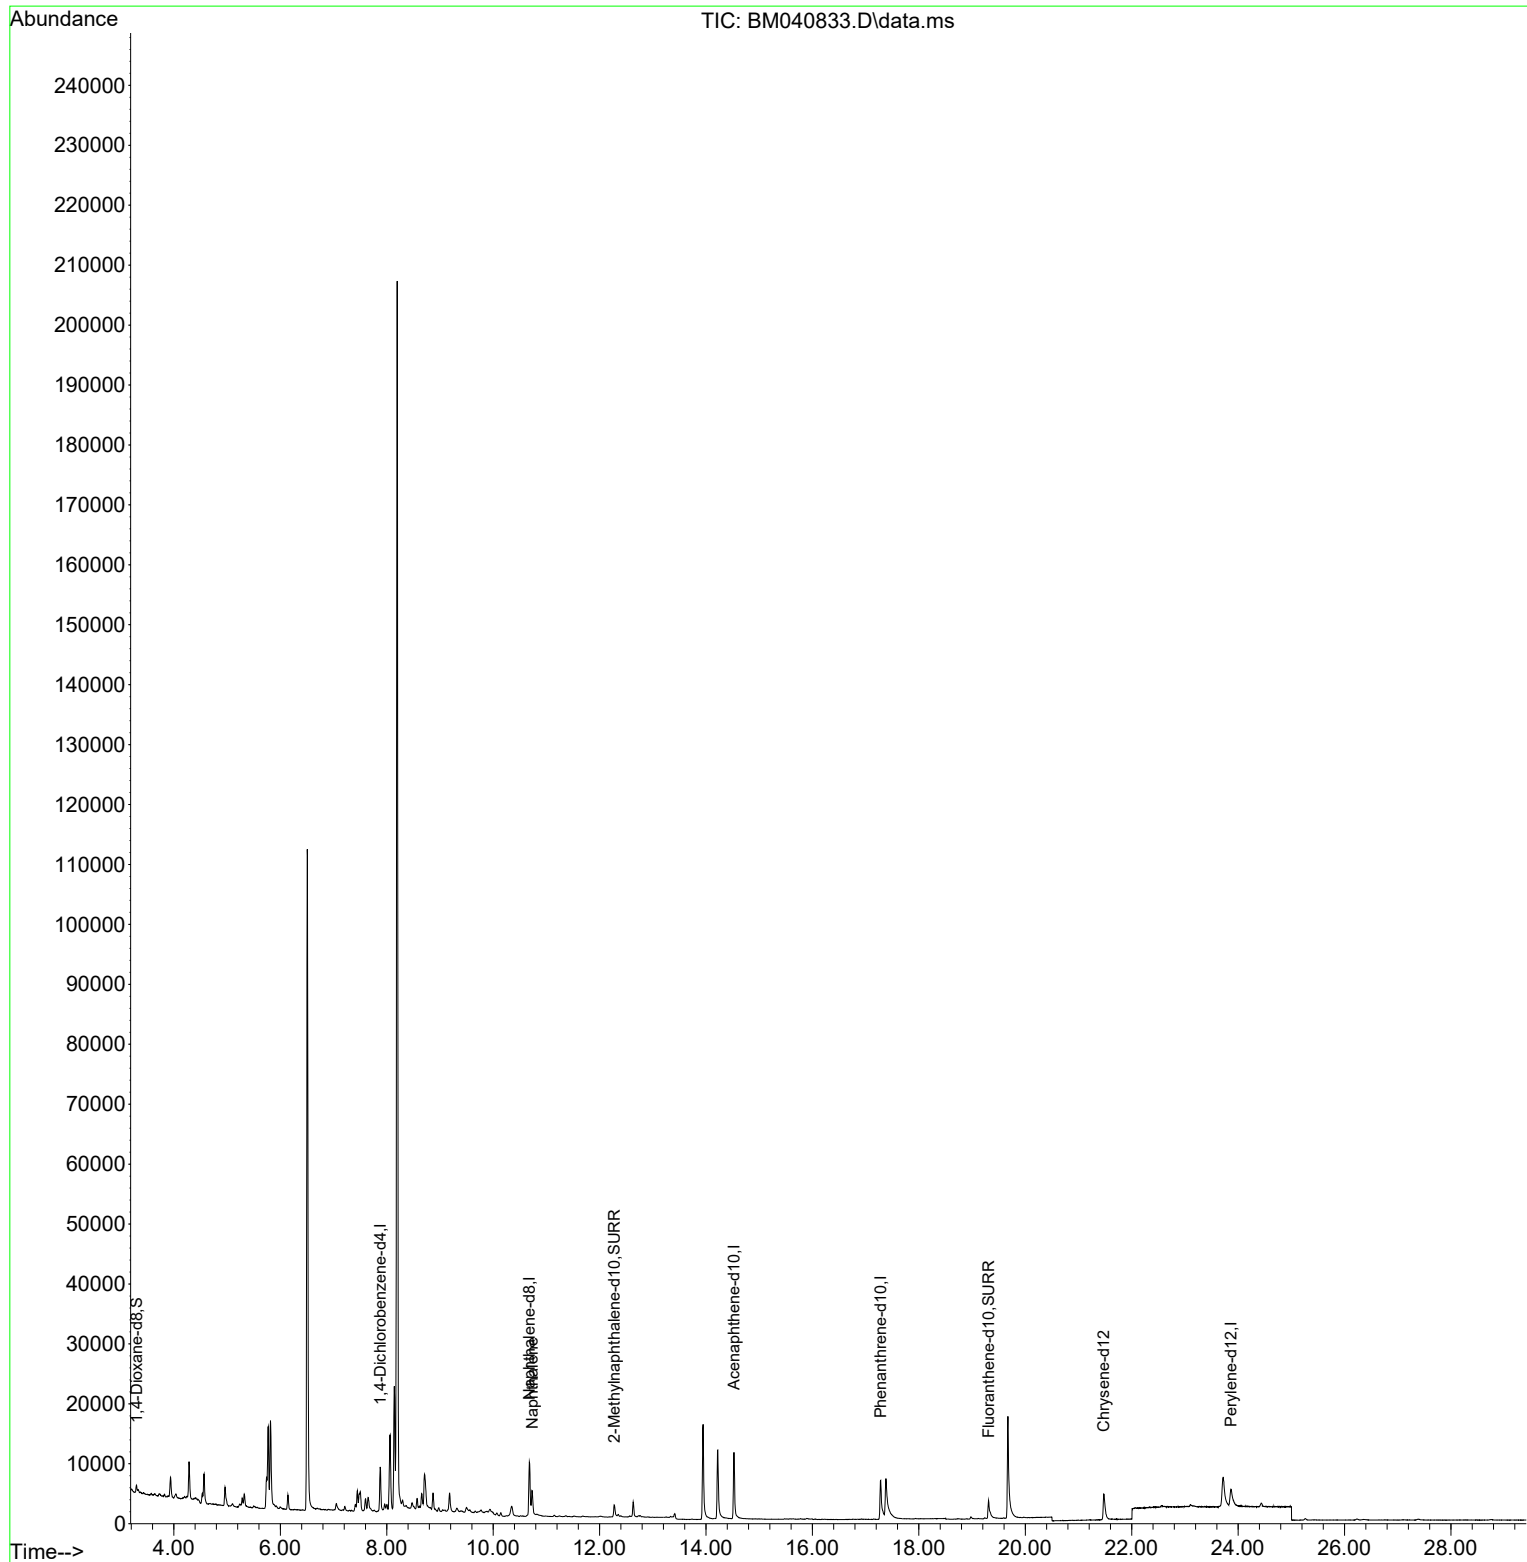

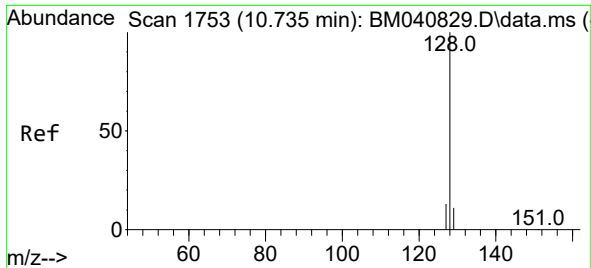

#5
Naphthalene
Concen: 0.159 ng/ul
RT: 10.735 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM040833.D
Acq: 12 Jul 2023 12:18

Instrument :
BNA_M
ClientSampleId :
A46G4

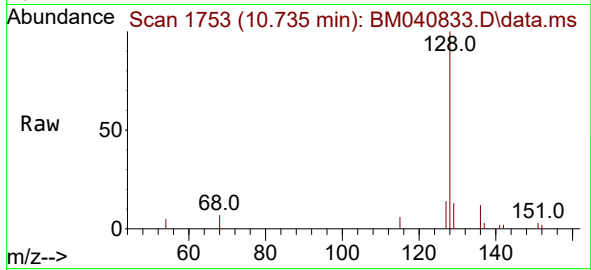

Tgt Ion:	128	Resp:	6616
Ion	Ratio	Lower	Upper
128	100		
129	13.5	9.2	13.8
127	14.4	10.6	15.8

